

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009412.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 09:03
Operator : AJ\MA
Sample : PB143591BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB143591BL

Integration File: autoint1.e
Quant Time: Mar 26 22:45:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	2513672	18.241 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009412.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 09:03
Operator : AJ\MA
Sample : PB143591BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB143591BL

Integration File: autoint1.e
Quant Time: Mar 26 22:45:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

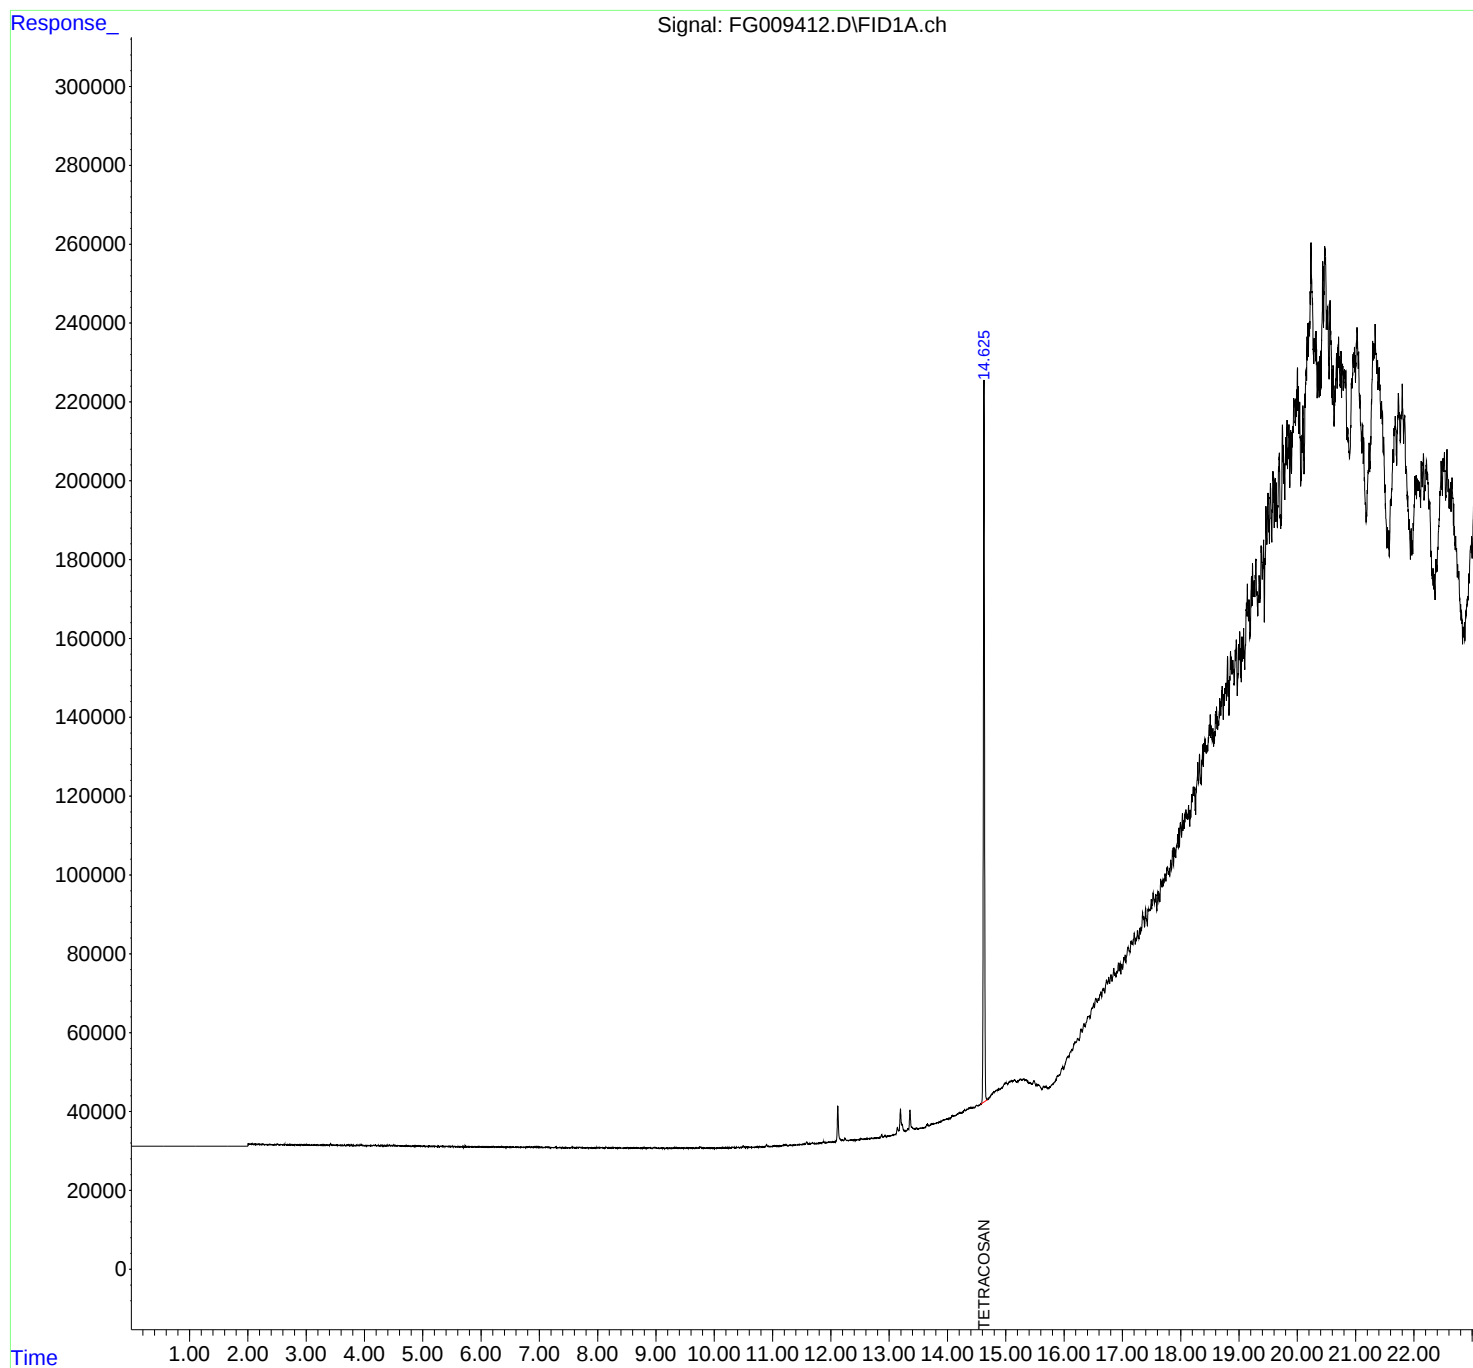

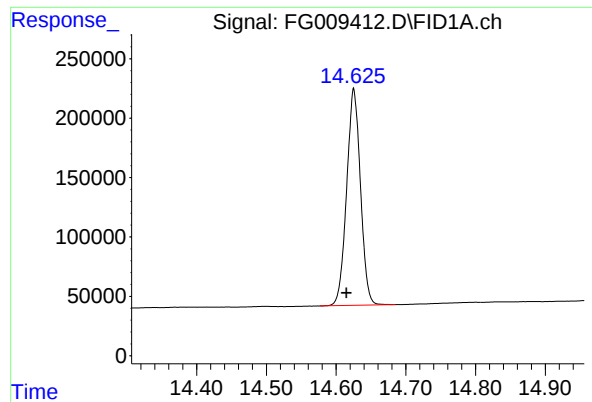

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.625 min
Delta R.T.: 0.010 min
Response: 2513672
Conc: 18.24 ug/ml

Instrument :
FID_G
ClientSampleId :
PB143591BL