

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
 Data File : FG009426.D
 Signal(s) : FID1A.ch
 Acq On : 26 Mar 2022 17:06
 Operator : AJ\MA
 Sample : N1966-04 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 G-1-4-5-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2022
 Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
 Quant Time: Mar 26 22:47:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
 Quant Title :
 QLast Update : Sat Mar 26 00:33:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	197706	1.435 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009426.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 17:06
Operator : AJ\MA
Sample : N1966-04 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
G-1-4-5-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
Quant Time: Mar 26 22:47:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

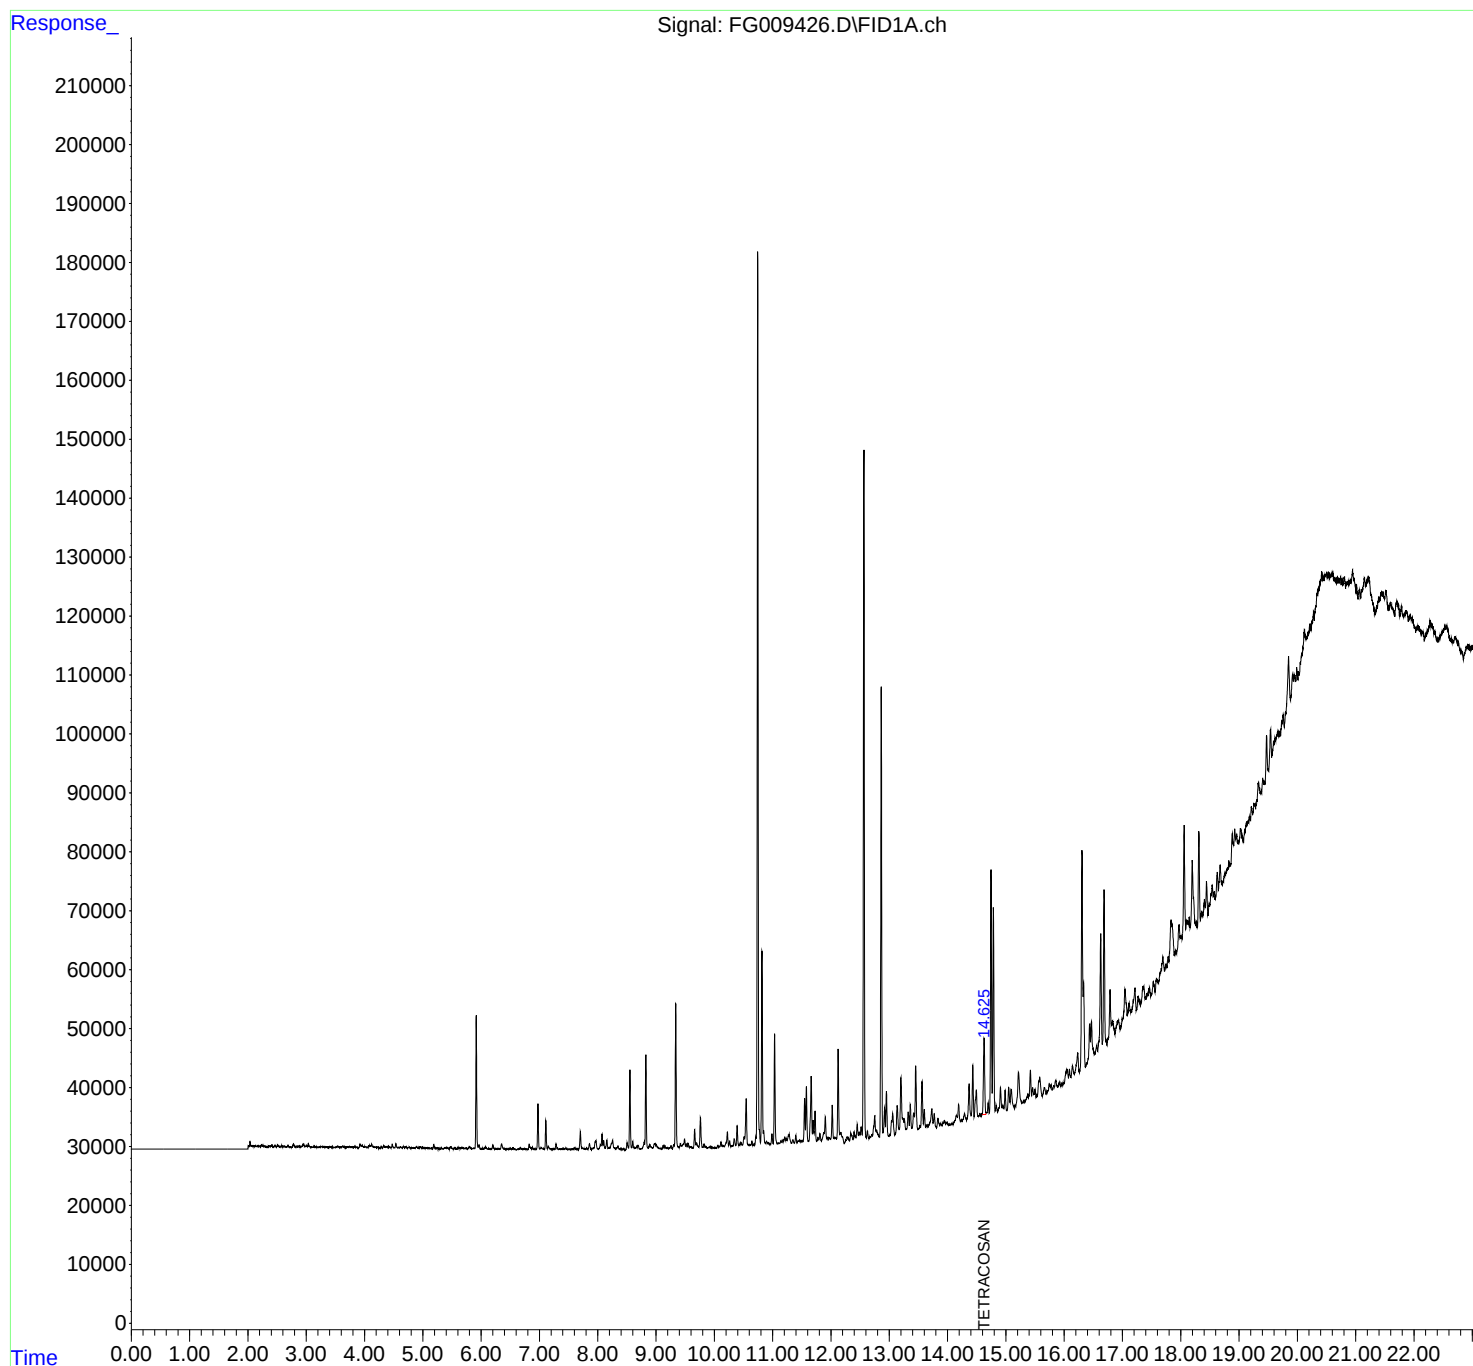

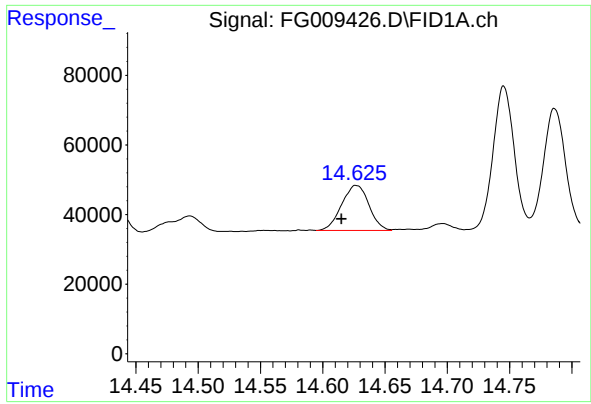

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.625 min
Delta R.T.: 0.011 min
Response: 197706
Conc: 1.43 ug/ml

Instrument :
FID_G
ClientSampleId :
G-1-4-5-6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/30/2022