

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009431.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 19:36
Operator : AJ\MA
Sample : N1966-05 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
G-1-5-9-10

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
Quant Time: Mar 26 22:47:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.626	158390	1.149 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009431.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 19:36
Operator : AJ\MA
Sample : N1966-05 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
G-1-5-9-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
Quant Time: Mar 26 22:47:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

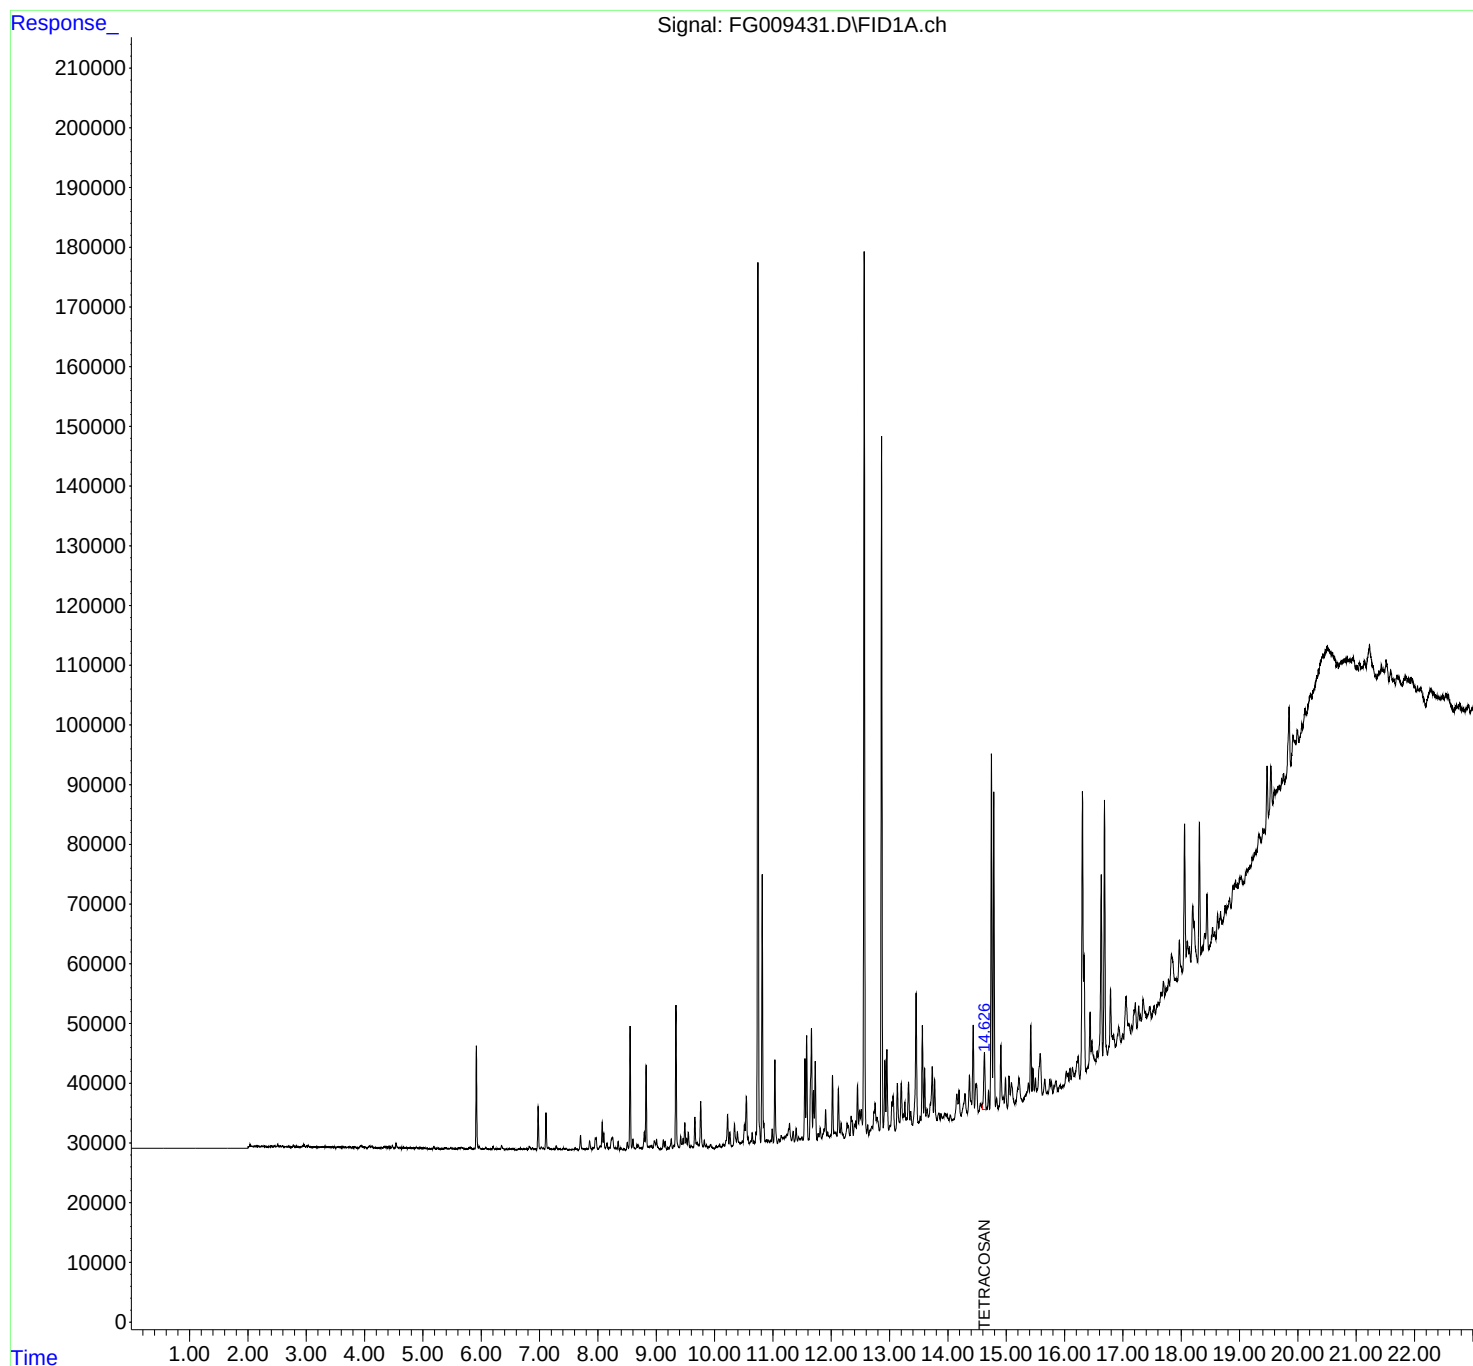

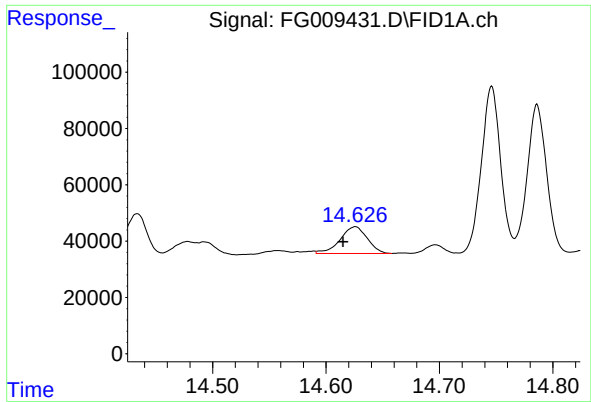

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.626 min
Delta R.T.: 0.011 min
Response: 158390
Conc: 1.15 ug/ml

Instrument :
FID_G
ClientSampleId :
G-1-5-9-10

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/30/2022