

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032719\
Data File : FG004370.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2019 15:14
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 28 01:05:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.176	2028822	19.257 ug/ml
12) N-OCTACOSANE	16.596	2383737	20.605 ug/ml
16) N-HEXATRIACONTANE	19.887	313474	2.812 ug/ml
18) N-TETRACONTANE	21.418	425077	3.930 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032719\
Data File : FG004370.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2019 15:14
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 28 01:05:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

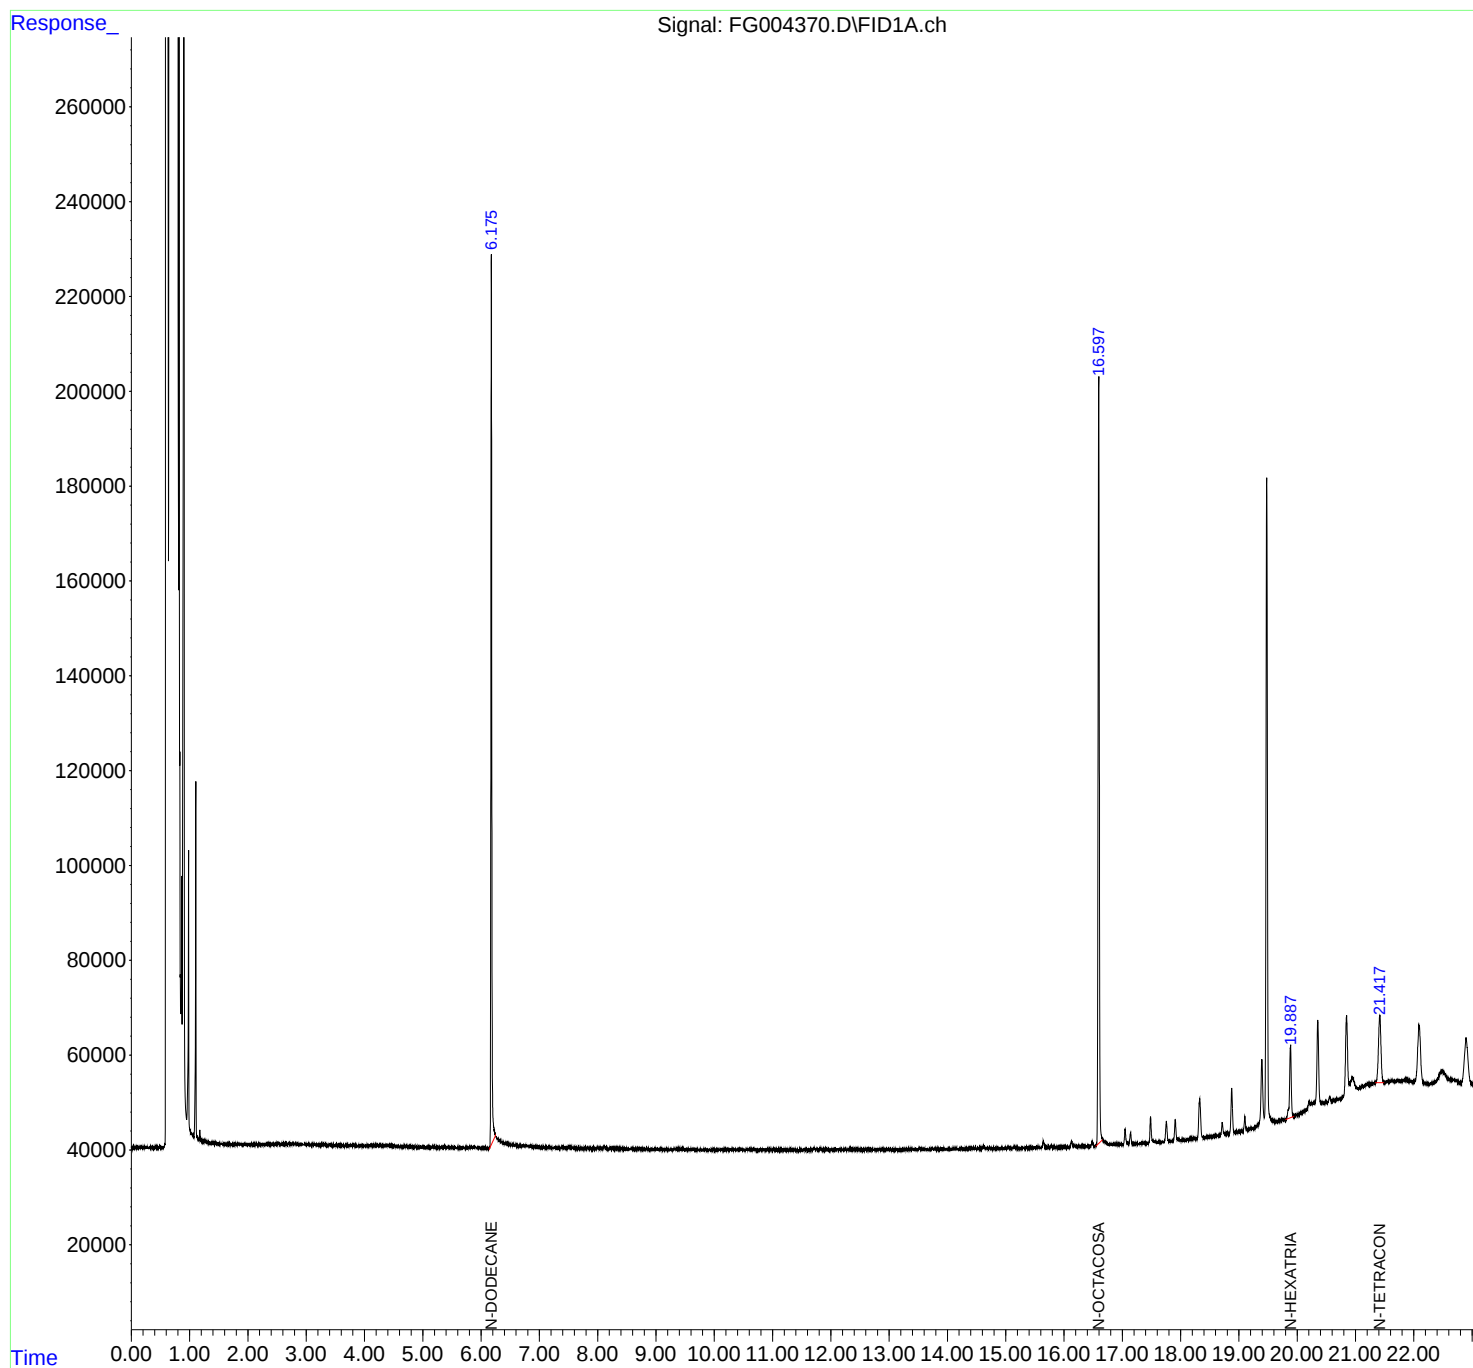


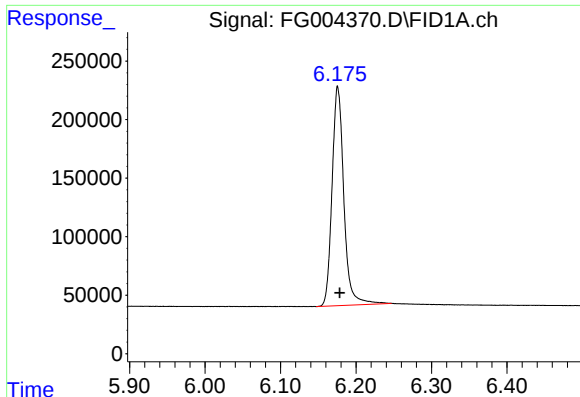

#3 N-DODECANE


R.T.: 6.176 min
Delta R.T.: -0.002 min
Response: 2028822
Conc: 19.26 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

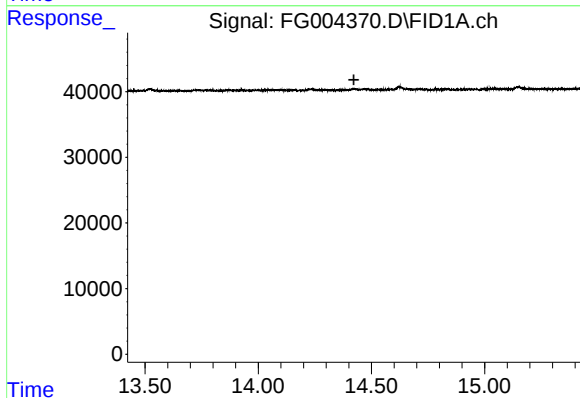


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

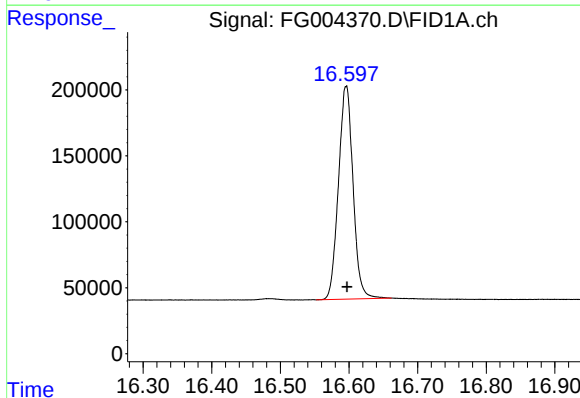


#12 N-OCTACOSANE

R.T.: 16.596 min
Delta R.T.: -0.001 min
Response: 2383737
Conc: 20.60 ug/ml

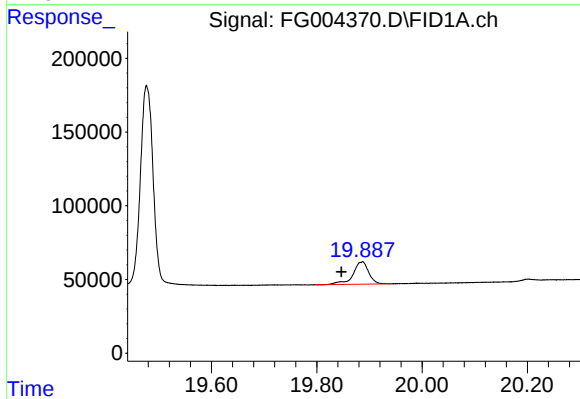

#16 N-HEXATRIACONTANE

R.T.: 19.887 min
Delta R.T.: 0.040 min
Response: 313474
Conc: 2.81 ug/ml

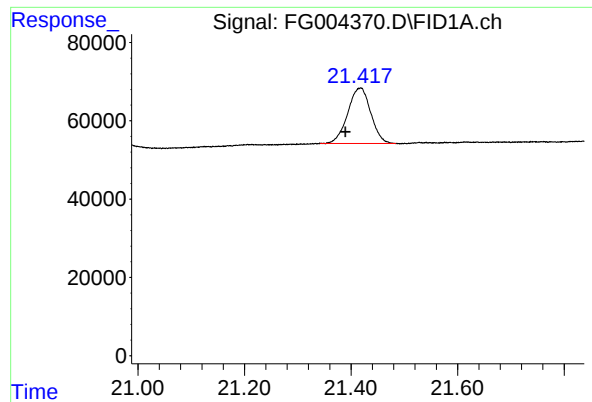

#18 N-TETRACONTANE

R.T.: 21.418 min
Delta R.T.: 0.029 min
Response: 425077
Conc: 3.93 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER