

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032719\
 Data File : FG004379.D
 Signal(s) : FID1A.ch
 Acq On : 27 Mar 2019 20:03
 Operator : AJ\SJ
 Sample : K2097-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 CS-22

Integration File: autoint1.e
 Quant Time: Mar 28 01:07:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.420	2593595	25.145 ug/ml
Target Compounds			
4) N-TETRADECANE	8.031f	401205	3.703 ug/ml
7) N-EICOSANE	12.369	1263262	11.051 ug/ml
10) N-TETRACOSANE	14.594	1545642	13.380 ug/ml
11) N-HEXACOSANE	15.647	227727	1.987 ug/ml
12) N-OCTACOSANE	16.595	422919	3.656 ug/ml
13) N-TRIACONTANE	17.481	387752	3.268 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032719\
Data File : FG004379.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2019 20:03
Operator : AJ\SJ
Sample : K2097-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CS-22

Integration File: autoint1.e
Quant Time: Mar 28 01:07:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

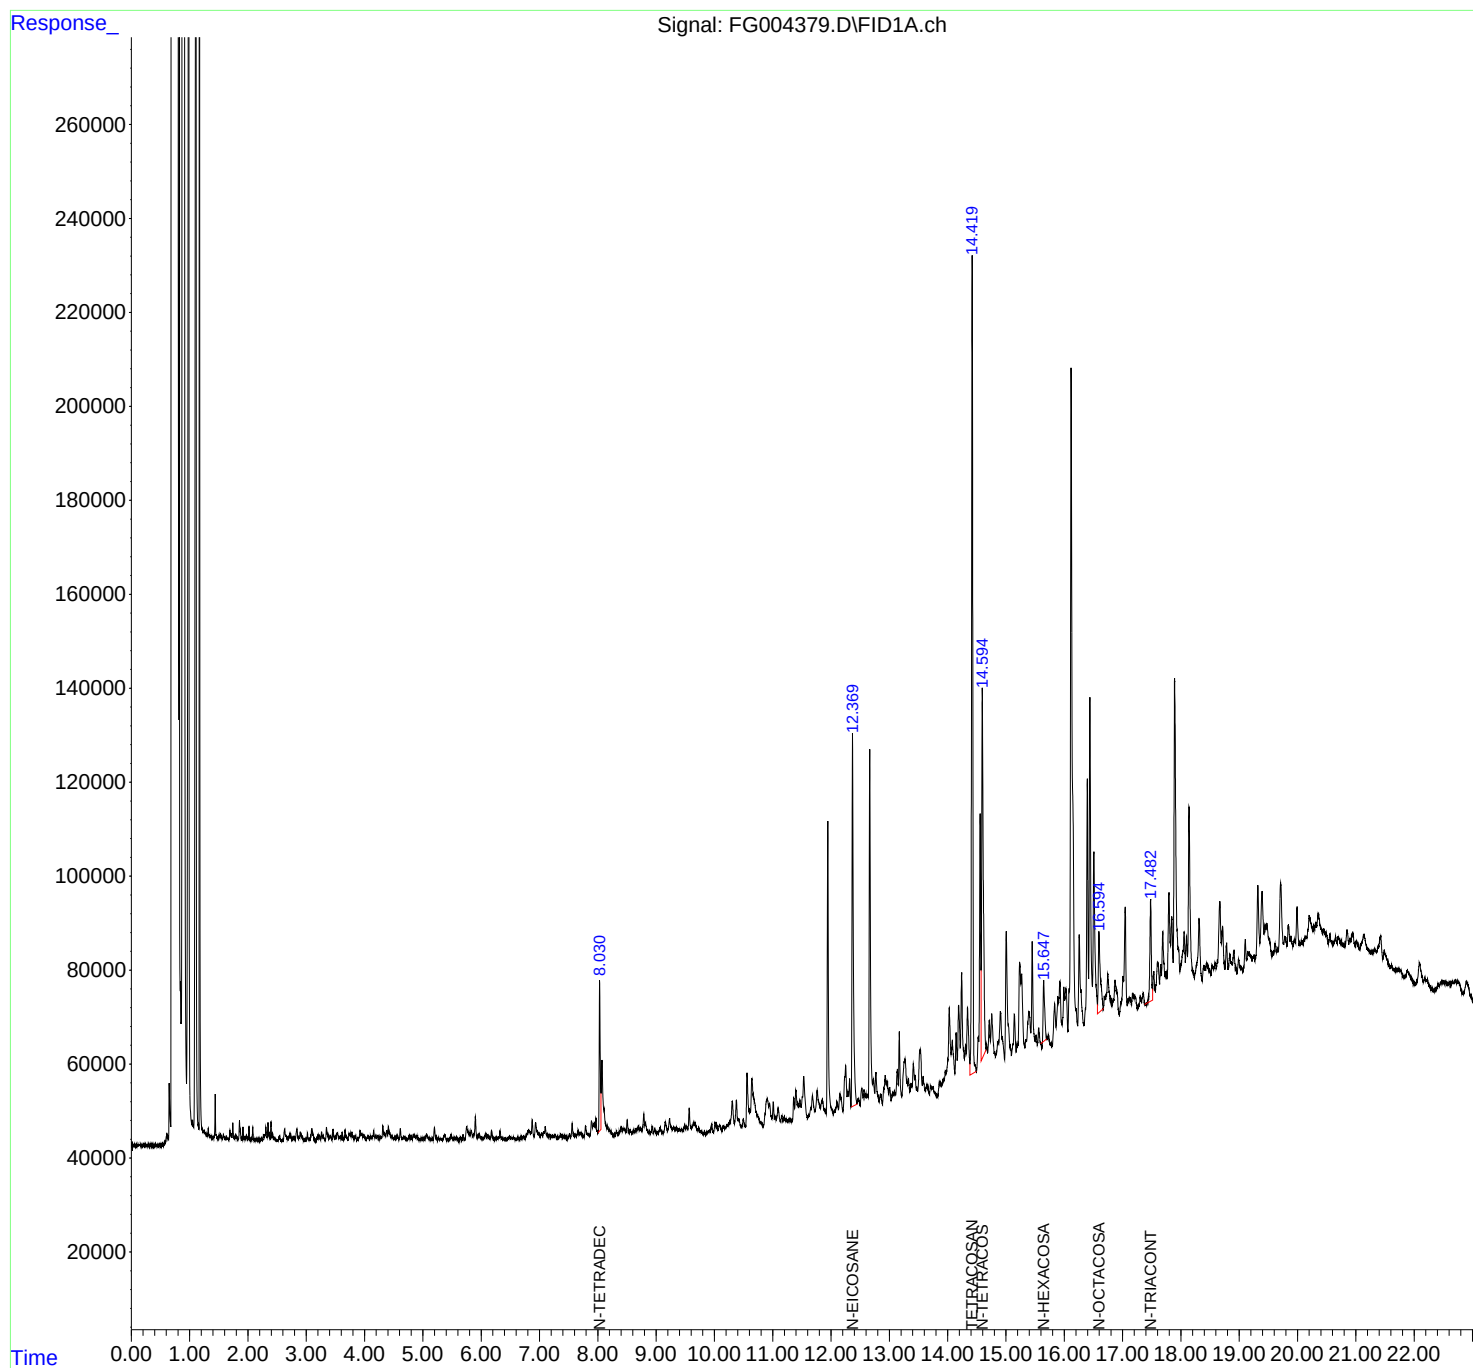


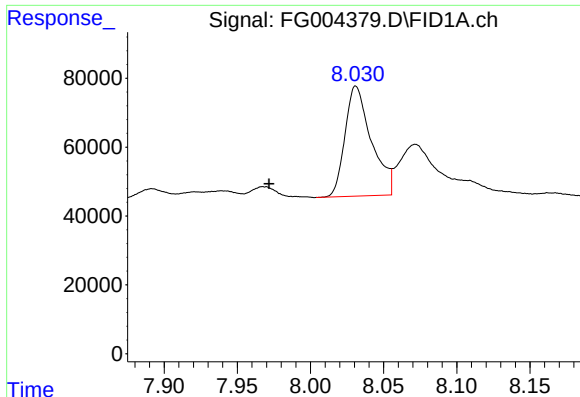

#4 N-TETRADECANE


R.T.: 8.031 min
Delta R.T.: 0.059 min
Response: 401205
Conc: 3.70 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-22

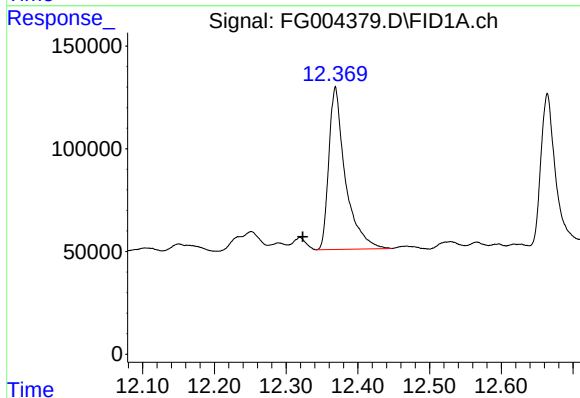


#7 N-EICOSANE

R.T.: 12.369 min
Delta R.T.: 0.046 min
Response: 1263262
Conc: 11.05 ug/ml

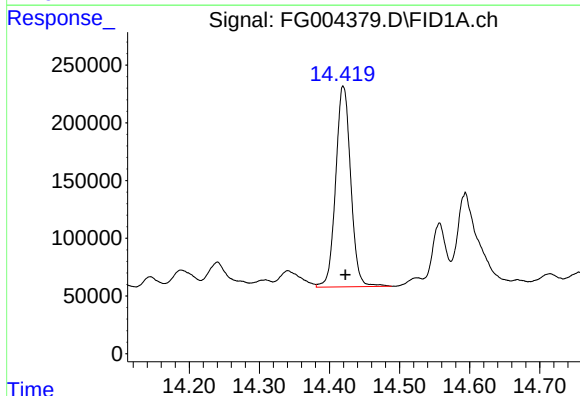


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.420 min
Delta R.T.: -0.003 min
Response: 2593595
Conc: 25.14 ug/ml

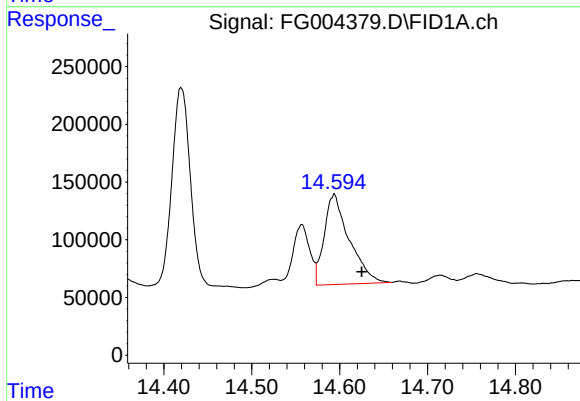

#10 N-TETRACOSANE


R.T.: 14.594 min
Delta R.T.: -0.031 min
Response: 1545642
Conc: 13.38 ug/ml

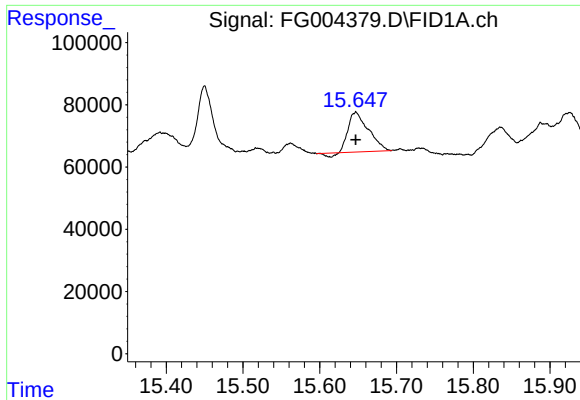

#11 N-HEXACOSANE


R.T.: 15.647 min
Delta R.T.: 0.000 min
Response: 227727
Conc: 1.99 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-22

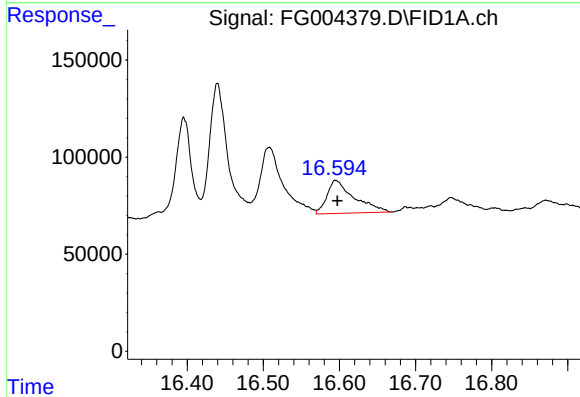

#12 N-OCTACOSANE

R.T.: 16.595 min
Delta R.T.: -0.003 min
Response: 422919
Conc: 3.66 ug/ml

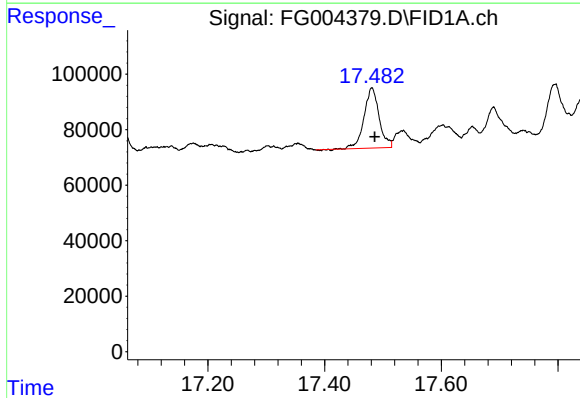

#13 N-TRIACONTANE

R.T.: 17.481 min
Delta R.T.: -0.005 min
Response: 387752
Conc: 3.27 ug/ml