

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032719\
 Data File : FG004374.D
 Signal(s) : FID1A.ch
 Acq On : 27 Mar 2019 17:29
 Operator : AJ\SJ
 Sample : PB118090BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB118090BS

Integration File: autoint1.e
 Quant Time: Mar 28 01:06:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.420	2049112	19.866 ug/ml
Target Compounds			
2) N-DECANE	4.155	2041961	19.345 ug/ml
3) N-DODECANE	6.176	2048487	19.443 ug/ml
4) N-TETRADECANE	7.969	2092875	19.316 ug/ml
5) N-HEXADECANE	9.569	2151130	19.227 ug/ml
6) N-OCTADECANE	11.010	2199369	19.390 ug/ml
7) N-EICOSANE	12.321	2227829	19.488 ug/ml
8) N-DOCOSANE	13.519	2225481	19.468 ug/ml
10) N-TETRACOSANE	14.622	2258740	19.553 ug/ml
11) N-HEXACOSANE	15.644	2246555	19.598 ug/ml
12) N-OCTACOSANE	16.594	2264124	19.571 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032719\
Data File : FG004374.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2019 17:29
Operator : AJ\SJ
Sample : PB118090BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB118090BS

Integration File: autoint1.e
Quant Time: Mar 28 01:06:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

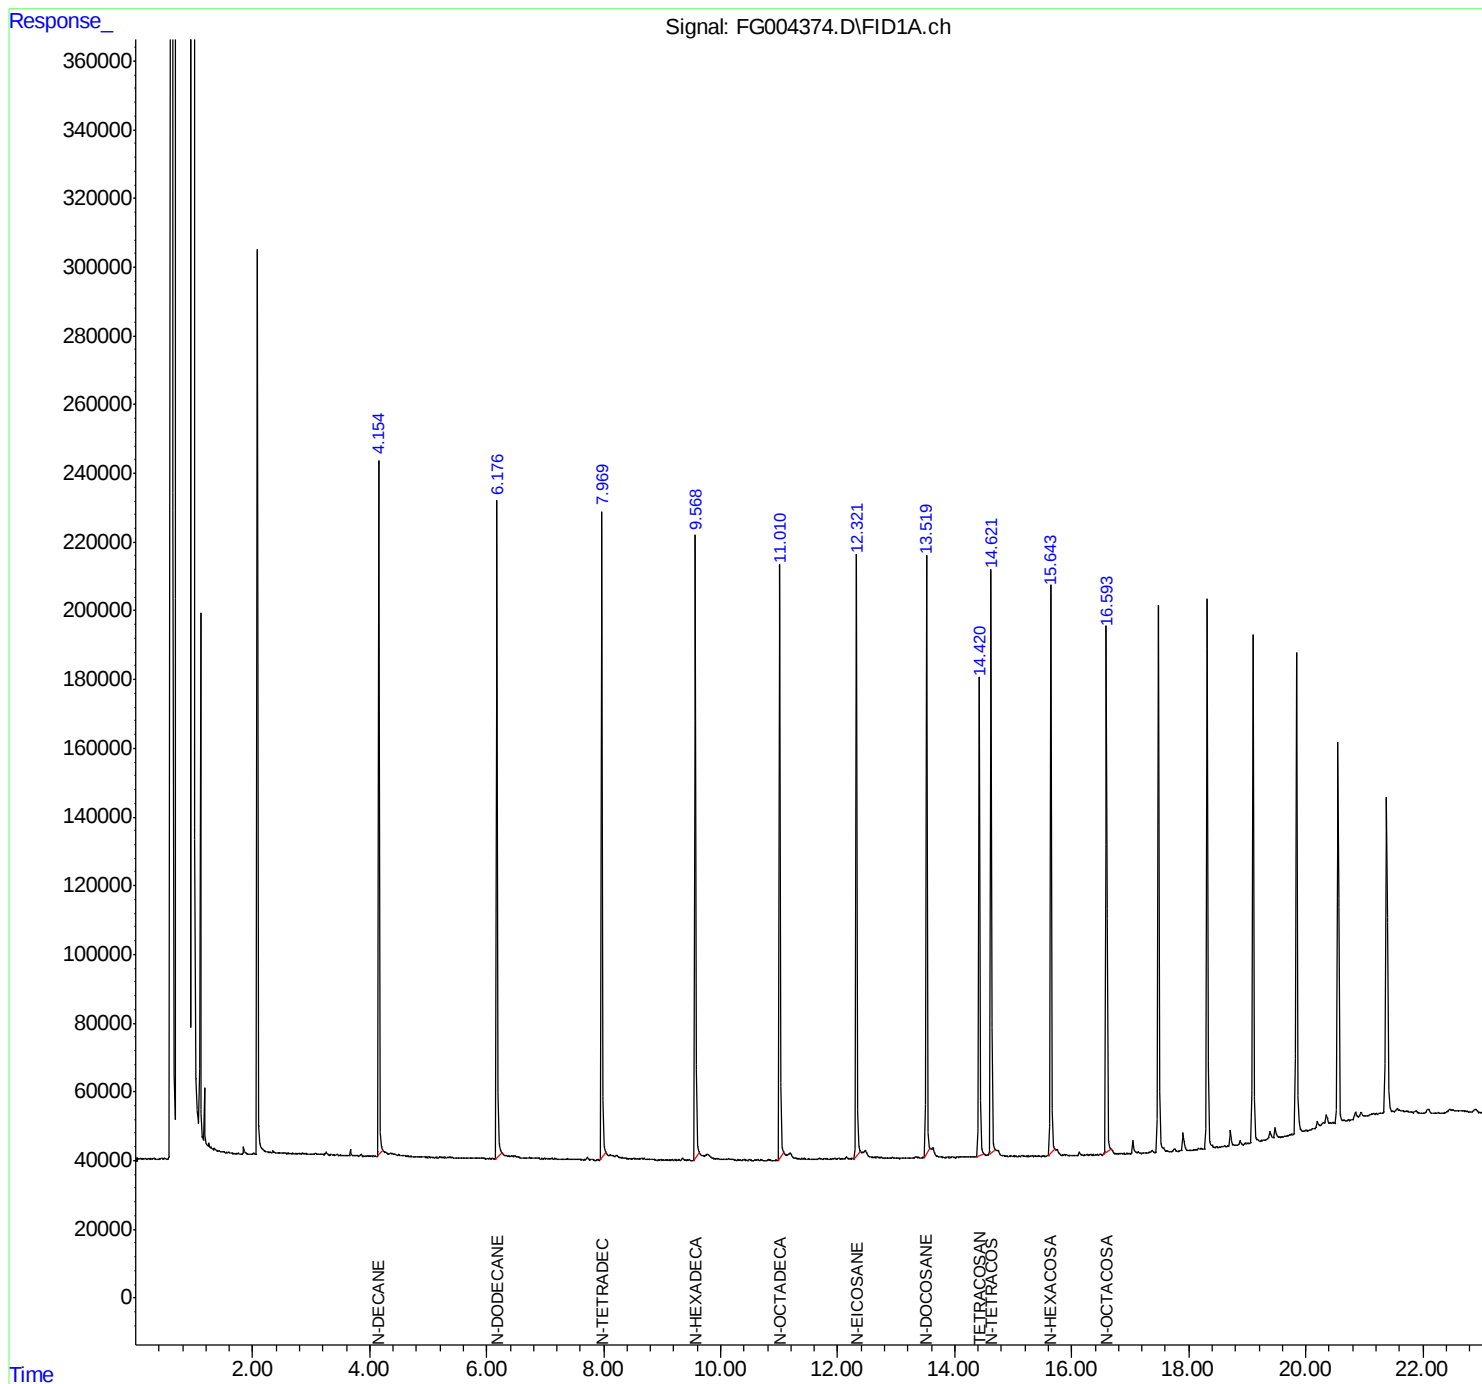


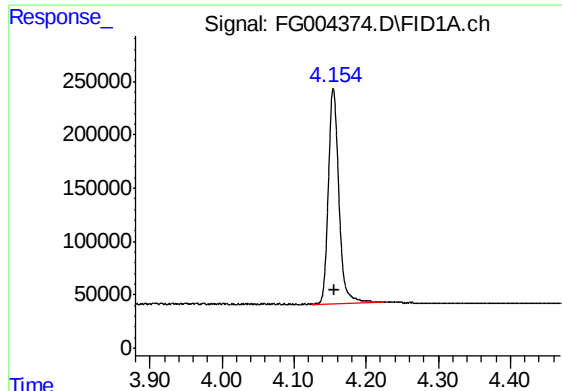

#2 N-DECANE


R.T.: 4.155 min
Delta R.T.: -0.002 min
Response: 2041961
Conc: 19.34 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118090BS

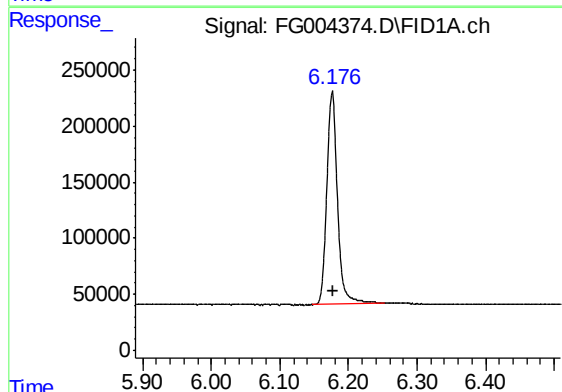


#3 N-DODECANE

R.T.: 6.176 min
Delta R.T.: -0.002 min
Response: 2048487
Conc: 19.44 ug/ml

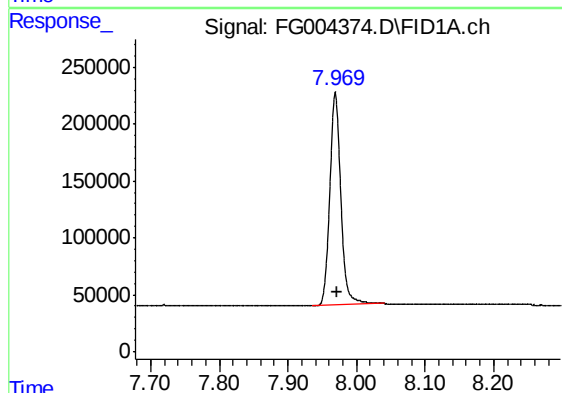


#4 N-TETRADECANE

R.T.: 7.969 min
Delta R.T.: -0.003 min
Response: 2092875
Conc: 19.32 ug/ml

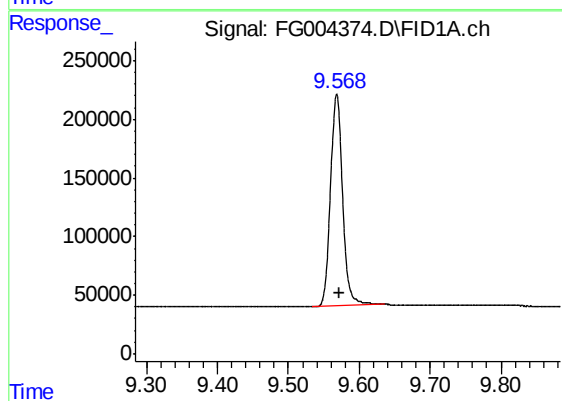

#5 N-HEXADECANE


R.T.: 9.569 min
Delta R.T.: -0.003 min
Response: 2151130
Conc: 19.23 ug/ml

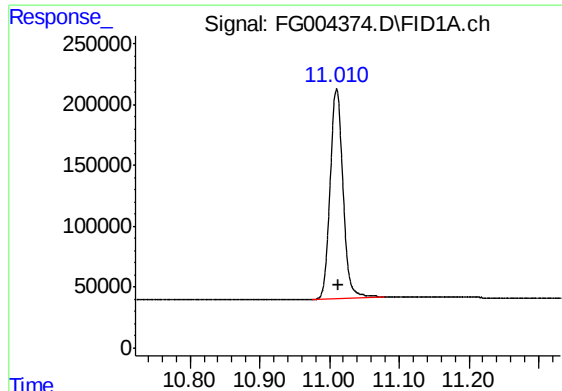

#6 N-OCTADECANE


R.T.: 11.010 min
Delta R.T.: -0.003 min
Response: 2199369
Conc: 19.39 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118090BS

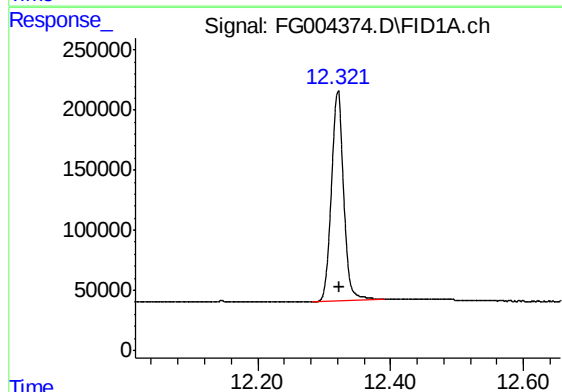


#7 N-EICOSANE

R.T.: 12.321 min
Delta R.T.: -0.002 min
Response: 2227829
Conc: 19.49 ug/ml

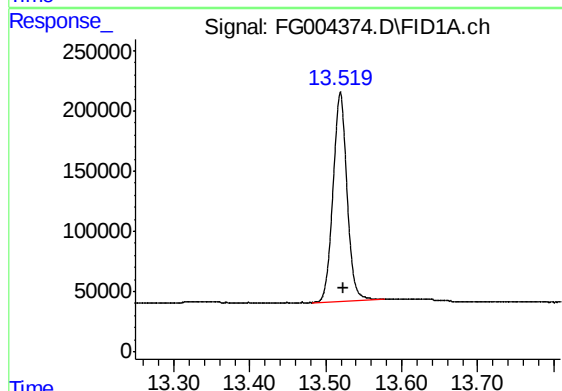


#8 N-DOCOSANE

R.T.: 13.519 min
Delta R.T.: -0.003 min
Response: 2225481
Conc: 19.47 ug/ml

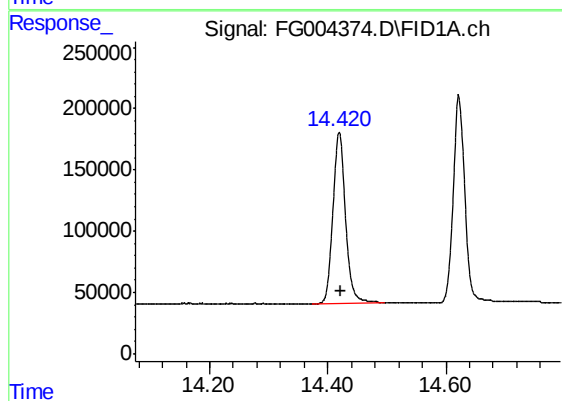

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.420 min
Delta R.T.: -0.003 min
Response: 2049112
Conc: 19.87 ug/ml

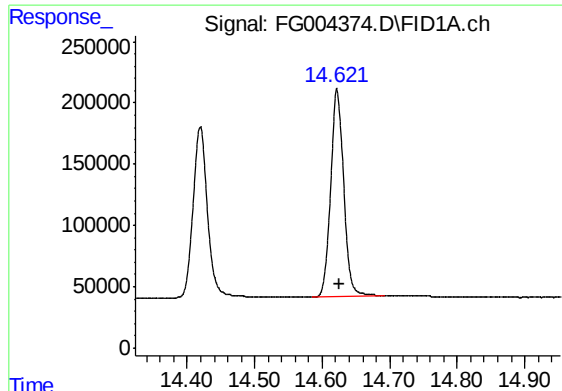

#10 N-TETRACOSANE


R.T.: 14.622 min
Delta R.T.: -0.003 min
Response: 2258740
Conc: 19.55 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118090BS

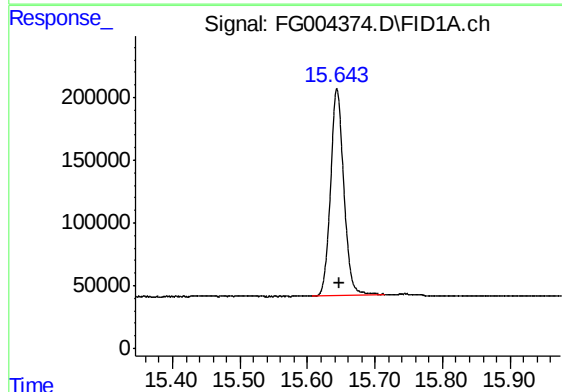

#11 N-HEXACOSANE

R.T.: 15.644 min
Delta R.T.: -0.003 min
Response: 2246555
Conc: 19.60 ug/ml

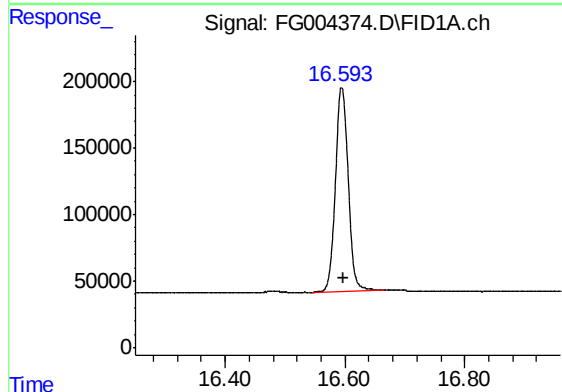

#12 N-OCTACOSANE

R.T.: 16.594 min
Delta R.T.: -0.003 min
Response: 2264124
Conc: 19.57 ug/ml