

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
Data File : FG011667.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2023 09:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 02:54:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.962	64005	0.690 ug/ml
15) N-TETRATRIACONTANE	19.737	61969	0.735 ug/ml
16) N-HEXATRIACONTANE	20.444	50183	0.652 ug/ml
17) N-OCTATRIACONTANE	21.237	220299	2.926 ug/ml
18) N-TETRACONTANE	22.232f	50407	0.687 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
Data File : FG011667.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2023 09:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 02:54:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

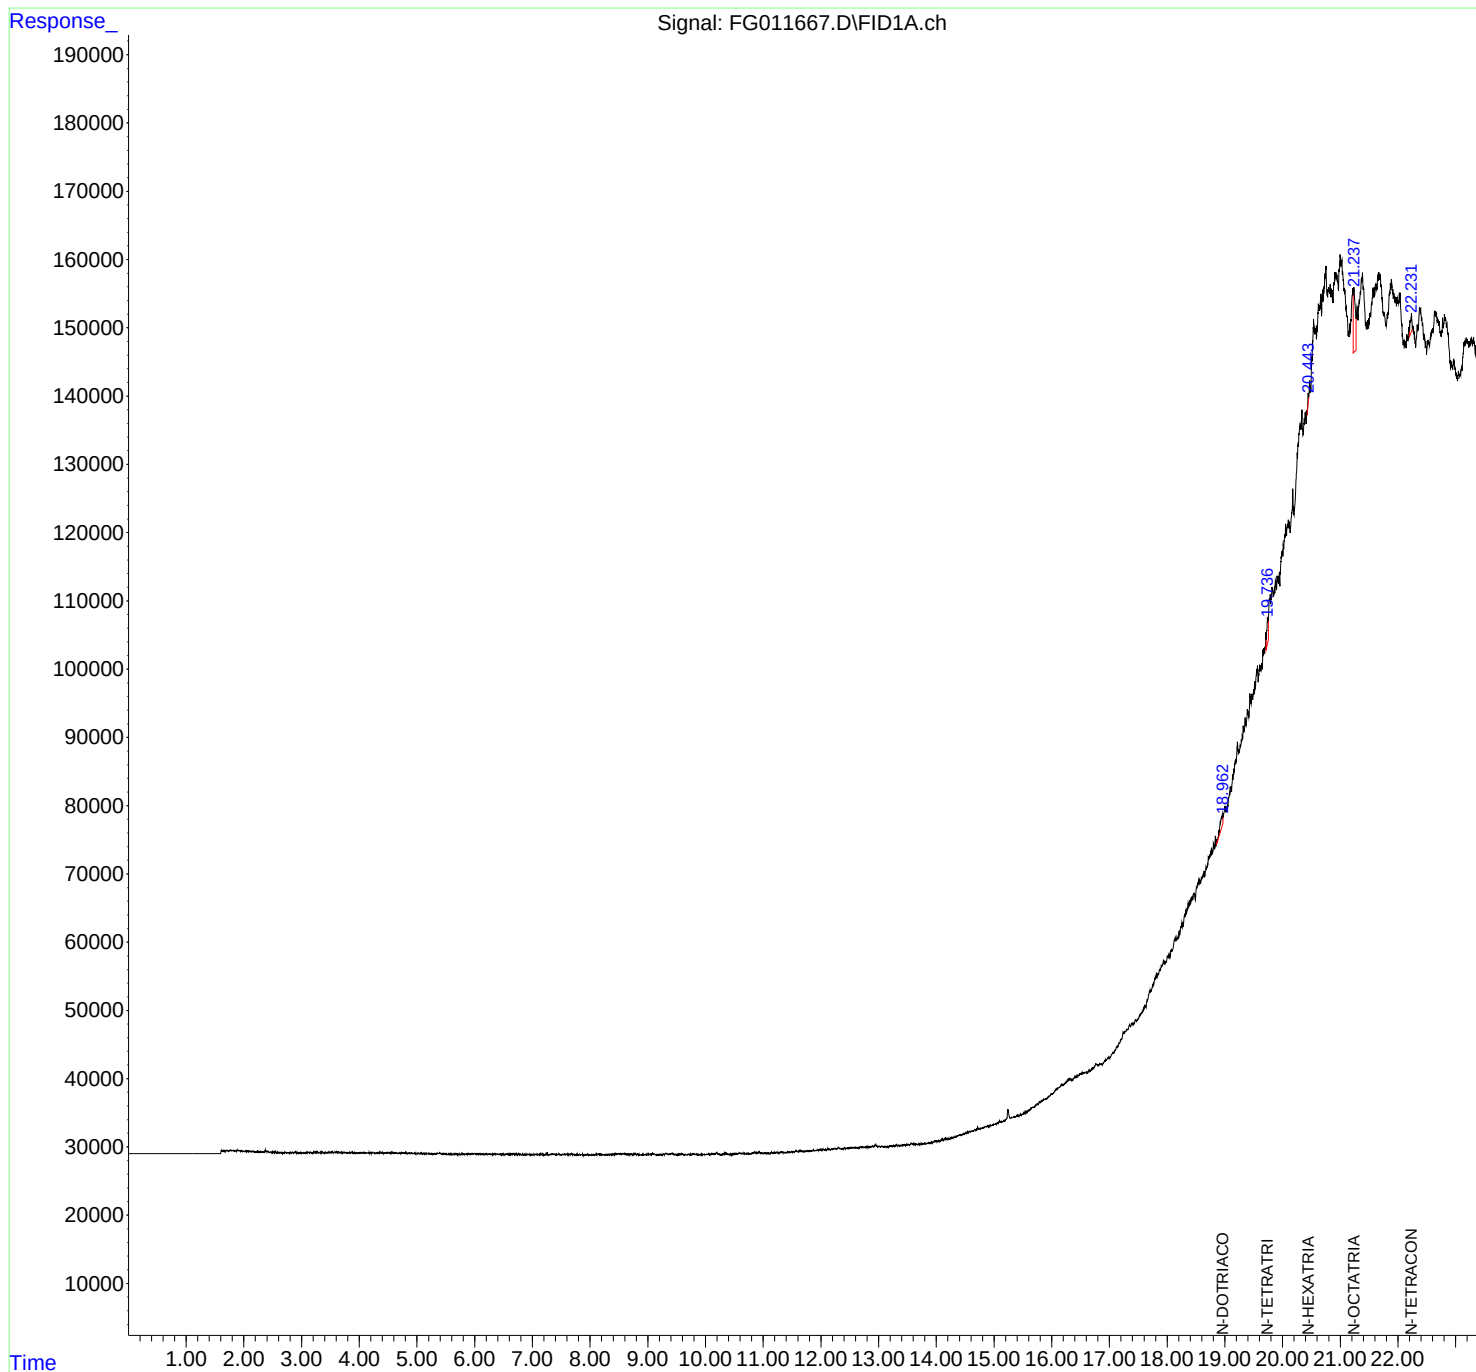


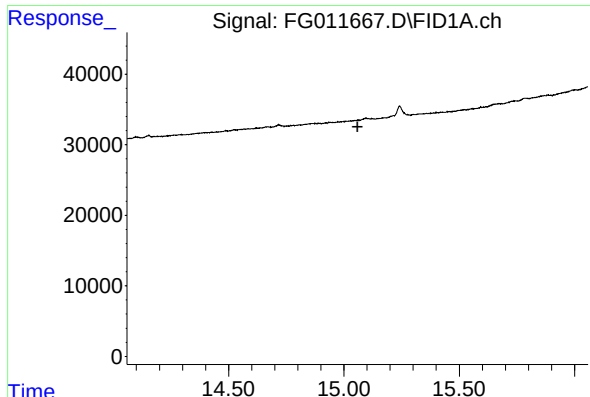

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.059 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

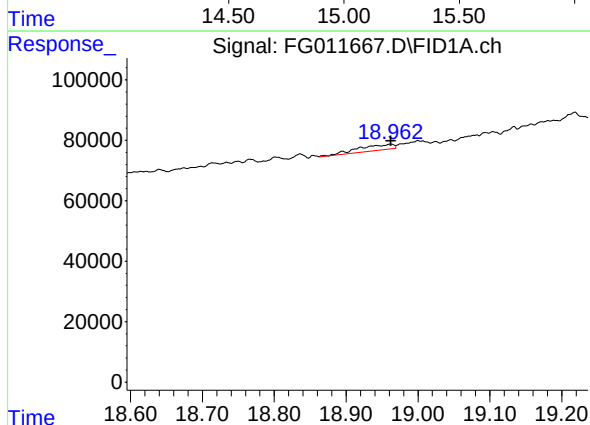


#14 N-DOTRIACONTANE

R.T.: 18.962 min
Delta R.T.: 0.000 min
Response: 64005
Conc: 0.69 ug/ml

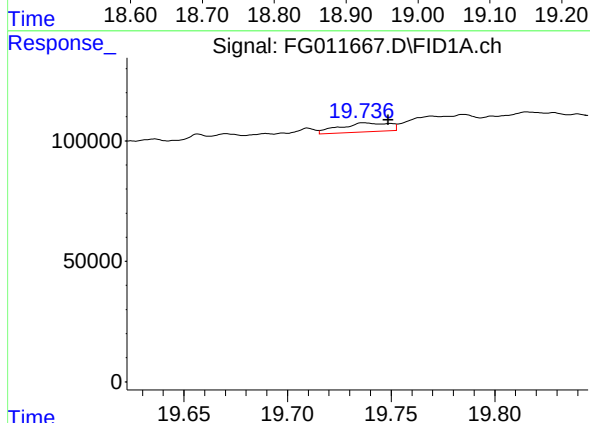


#15 N-TETRATRIACONTANE

R.T.: 19.737 min
Delta R.T.: -0.012 min
Response: 61969
Conc: 0.74 ug/ml

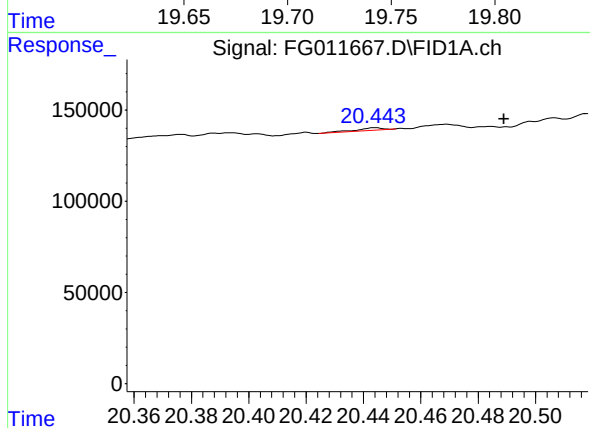

#16 N-HEXATRIACONTANE

R.T.: 20.444 min
Delta R.T.: -0.045 min
Response: 50183
Conc: 0.65 ug/ml

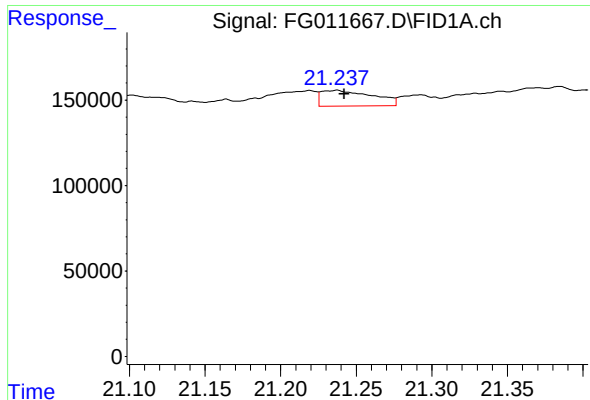


#17 N-OCTATRIACONTANE

R.T.: 21.237 min
Delta R.T.: -0.005 min
Response: 220299
Conc: 2.93 ug/ml

Instrument :

FID_G

ClientSampleId :

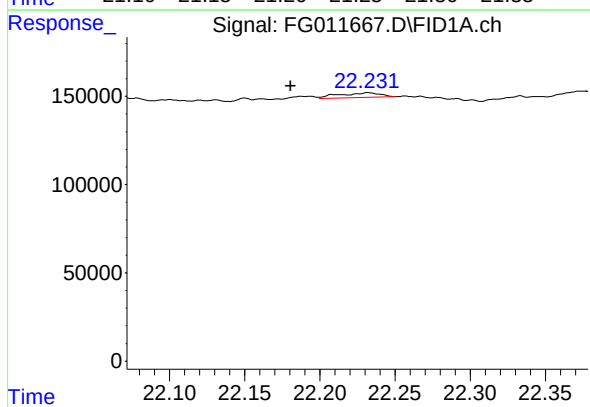

#18 N-TETRACONTANE

R.T.: 22.232 min
Delta R.T.: 0.052 min
Response: 50407
Conc: 0.69 ug/ml