

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
 Data File : FG011673.D
 Signal(s) : FID1A.ch
 Acq On : 27 Mar 2023 12:34
 Operator : YP\AJ
 Sample : 02090-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 28 02:55:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
 Quant Title :
 QLast Update : Wed Mar 15 18:43:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.053	2015539	20.025 ug/ml
Target Compounds			
17) N-OCTATRIACONTANE	21.214	394640	5.242 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
Data File : FG011673.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2023 12:34
Operator : YP\AJ
Sample : 02090-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 02:55:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

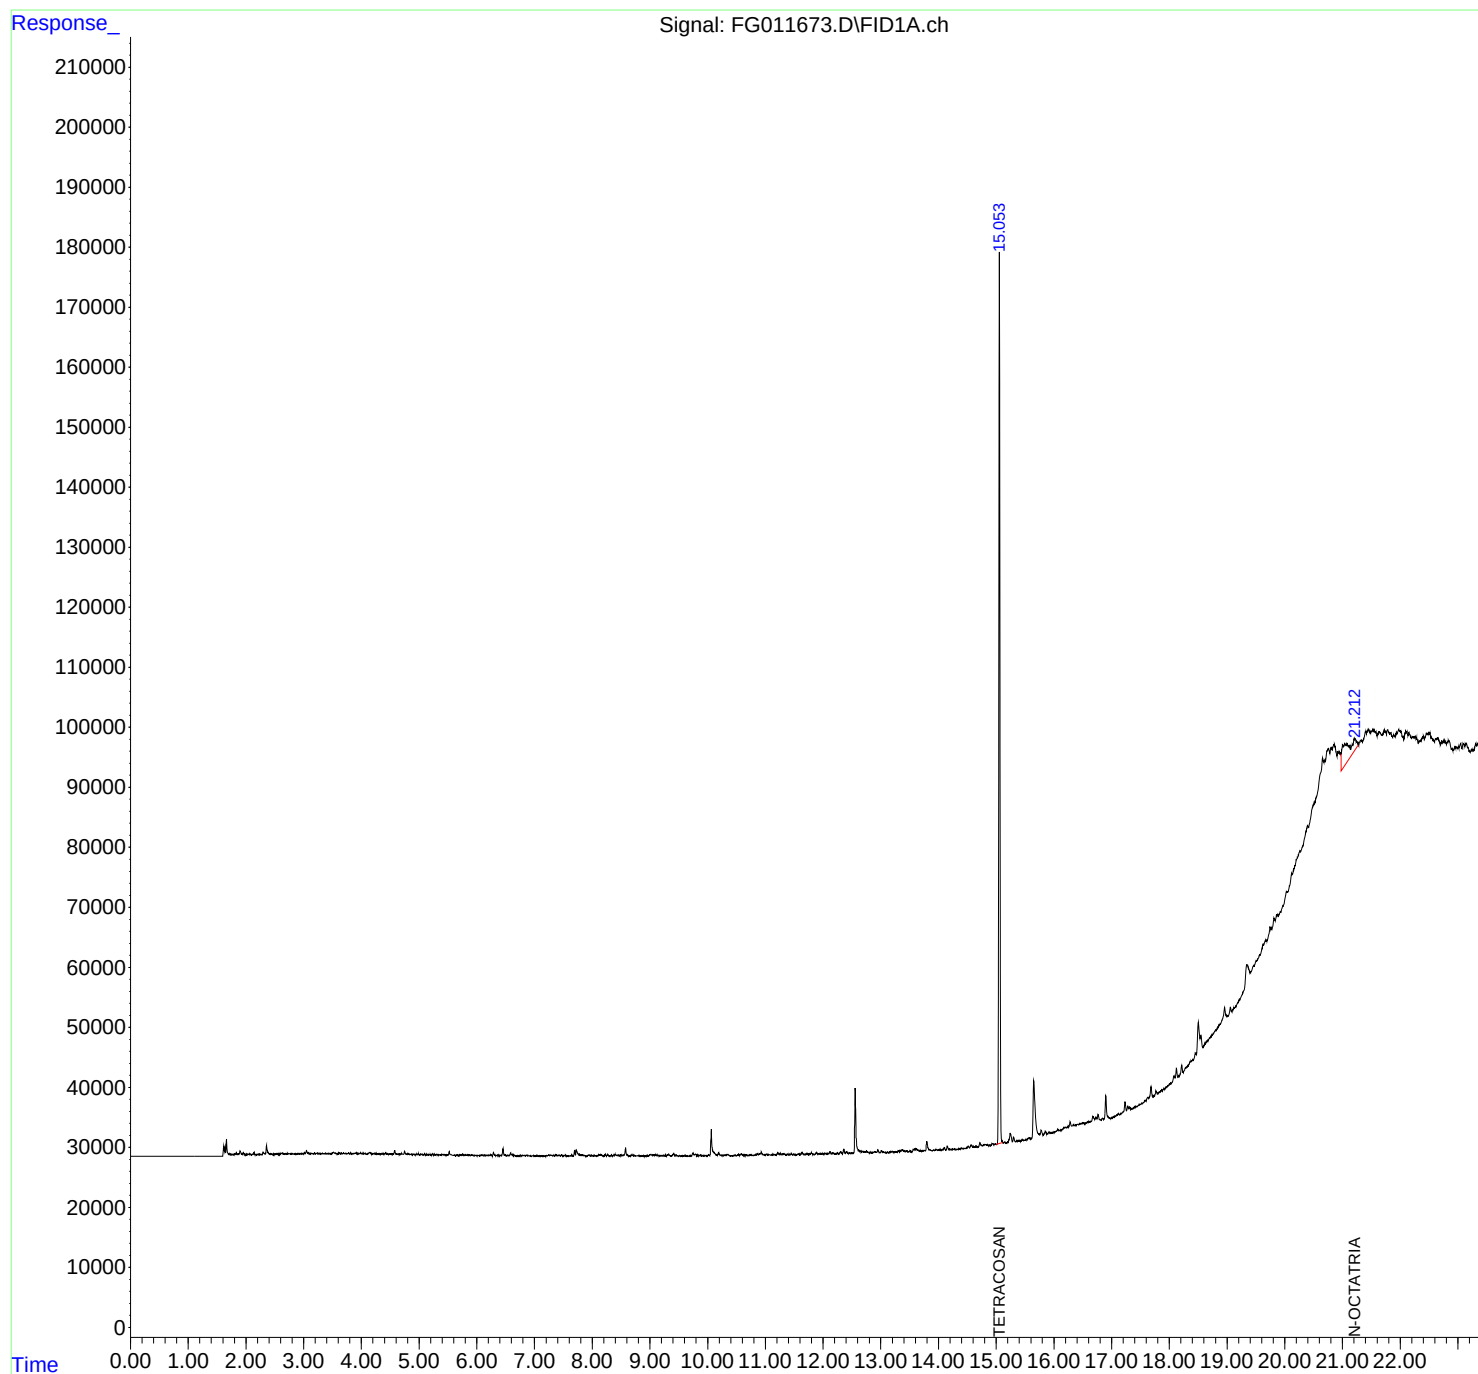

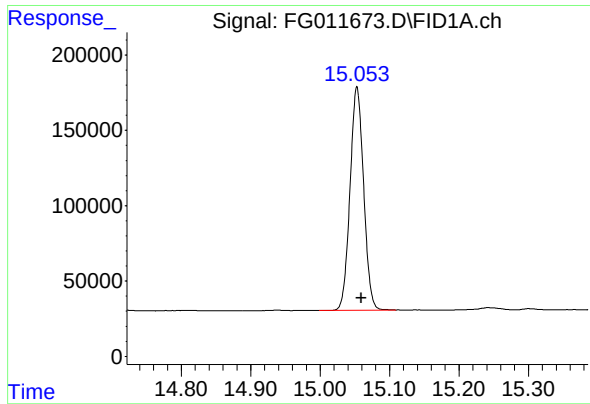


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.053 min
Delta R.T.: -0.006 min
Response: 2015539
Conc: 20.02 ug/ml

Instrument :

FID_G

ClientSampleId :

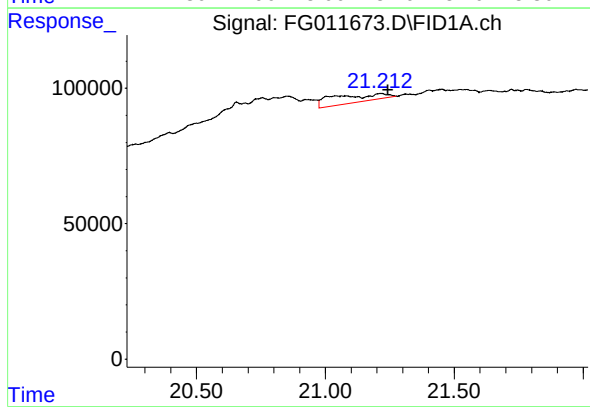

#17 N-OCTATRIACONTANE

R.T.: 21.214 min
Delta R.T.: -0.028 min
Response: 394640
Conc: 5.24 ug/ml