

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
Data File : FG011674.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2023 13:04
Operator : YP\AJ
Sample : 02090-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DS-01-032323

Integration File: autoint1.e
Quant Time: Mar 28 02:55:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.053	2003944	19.909 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
Data File : FG011674.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2023 13:04
Operator : YP\AJ
Sample : 02090-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DS-01-032323

Integration File: autoint1.e
Quant Time: Mar 28 02:55:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

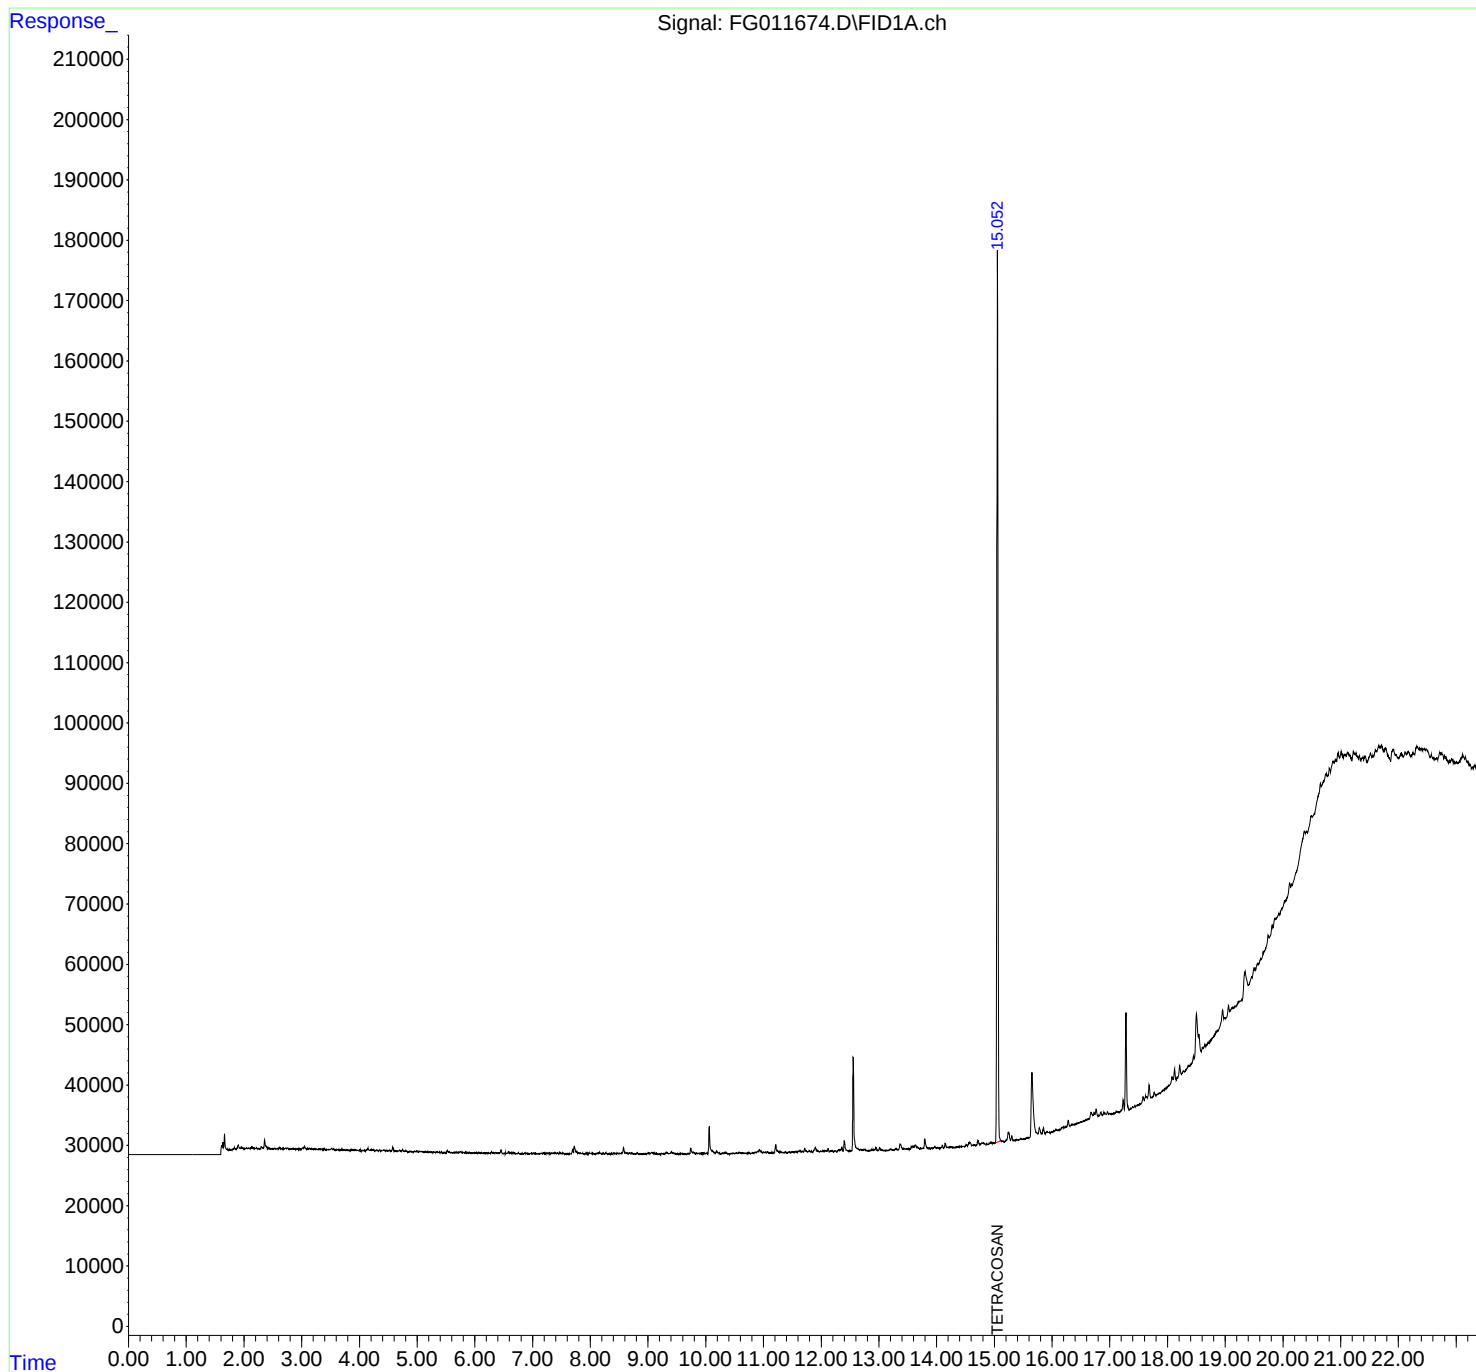

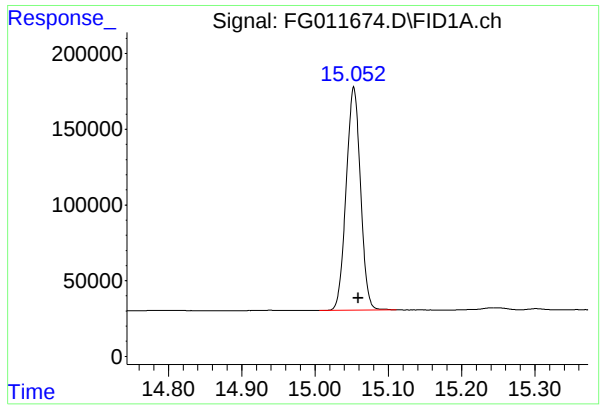

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.053 min
Delta R.T.: -0.006 min
Response: 2003944
Conc: 19.91 ug/ml

Instrument :
FID_G
ClientSampleId :
DS-01-032323