

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
Data File : FG011675.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2023 13:34
Operator : YP\AJ
Sample : PB151692BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB151692BL

Integration File: autoint1.e
Quant Time: Mar 28 02:55:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.053	1853987	18.419 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032723\
Data File : FG011675.D
Signal(s) : FID1A.ch
Acq On : 27 Mar 2023 13:34
Operator : YP\AJ
Sample : PB151692BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB151692BL

Integration File: autoint1.e
Quant Time: Mar 28 02:55:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

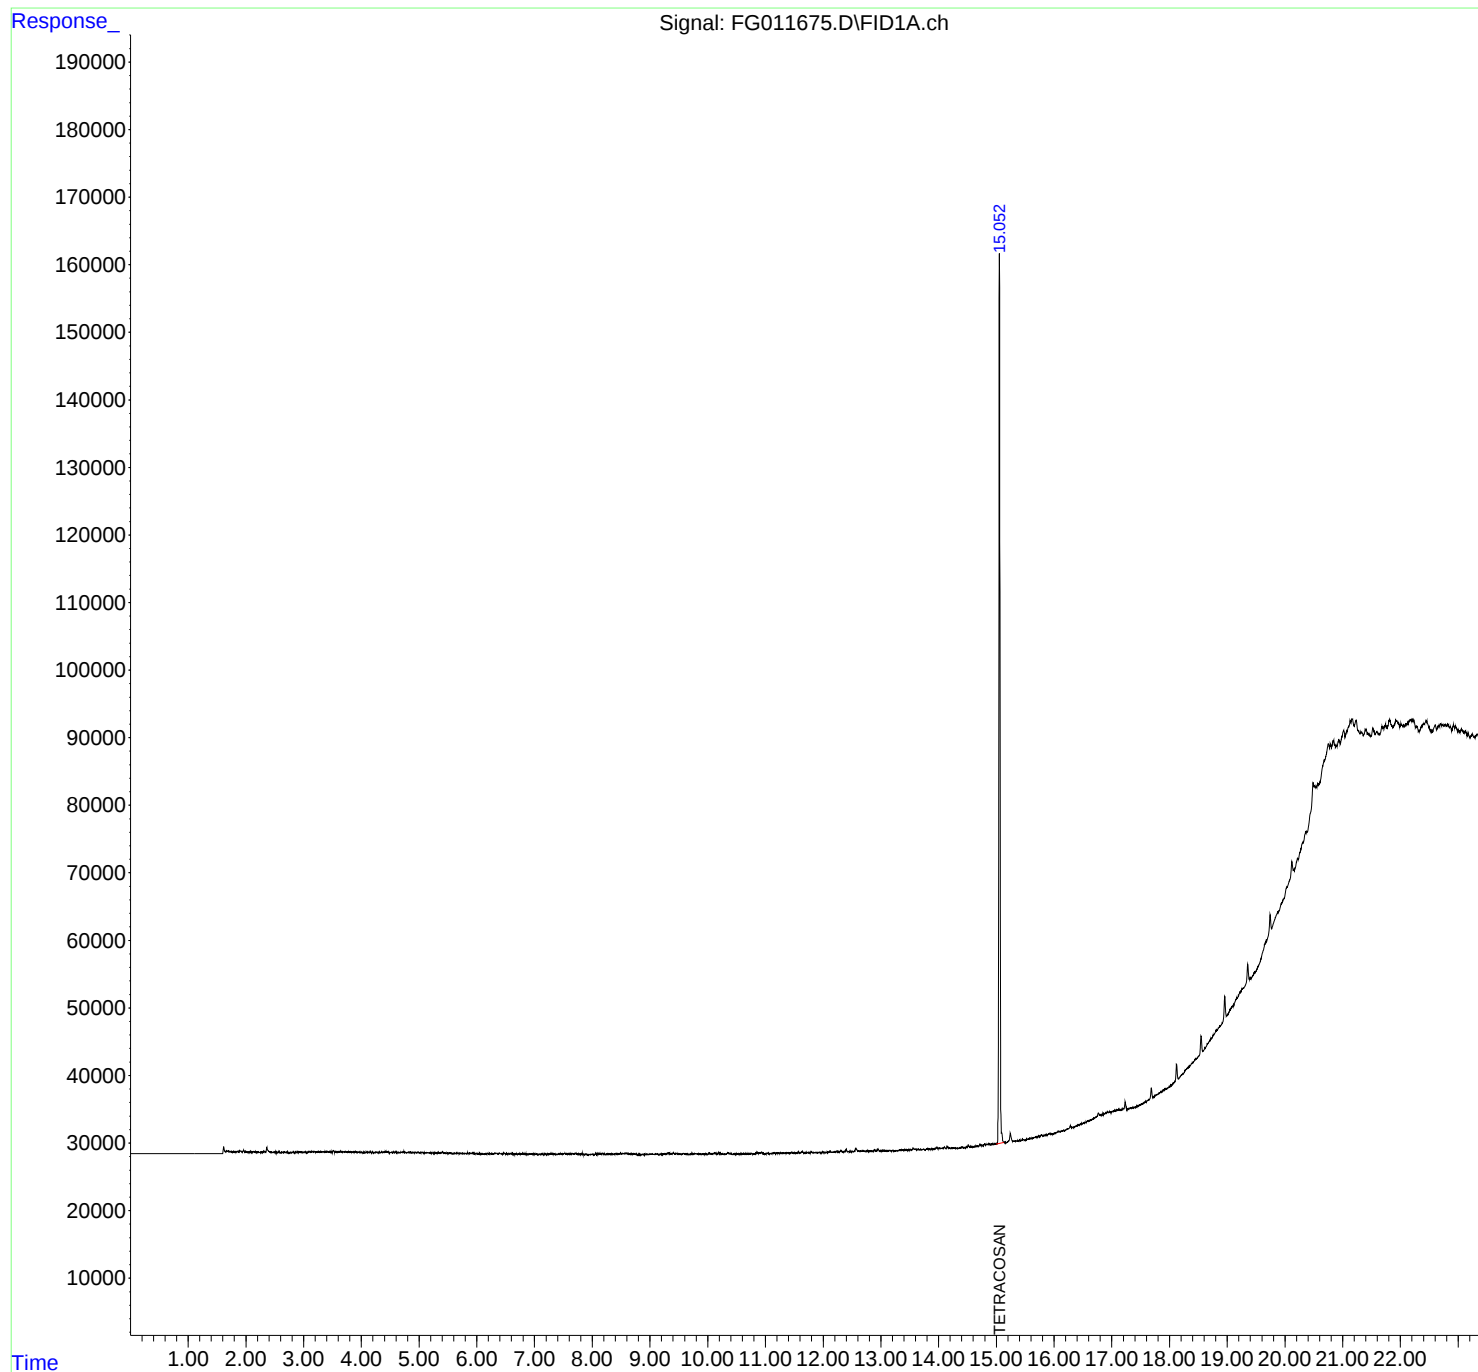

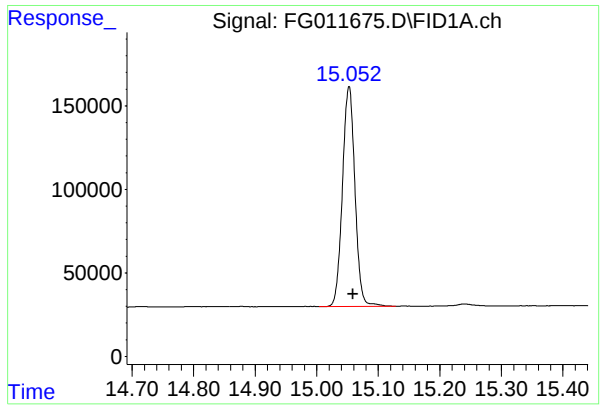

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.053 min
Delta R.T.: -0.006 min
Response: 1853987
Conc: 18.42 ug/ml

Instrument :
FID_G
ClientSampleId :
PB151692BL