

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032819\
 Data File : FG004393.D
 Signal(s) : FID1A.ch
 Acq On : 28 Mar 2019 12:13
 Operator : AJ\SJ
 Sample : K2097-02 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 CS-21

Integration File: autoint1.e
 Quant Time: Mar 29 03:42:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.421	860863	8.346 ug/ml
Target Compounds			
2) N-DECANE	4.154	158080	1.498 ug/ml
7) N-EICOSANE	12.372	1074181	9.397 ug/ml
10) N-TETRACOSANE	14.597	1272576	11.016 ug/ml
13) N-TRIACONTANE	17.483	221011	1.863 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032819\
Data File : FG004393.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2019 12:13
Operator : AJ\SJ
Sample : K2097-02 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CS-21

Integration File: autoint1.e
Quant Time: Mar 29 03:42:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

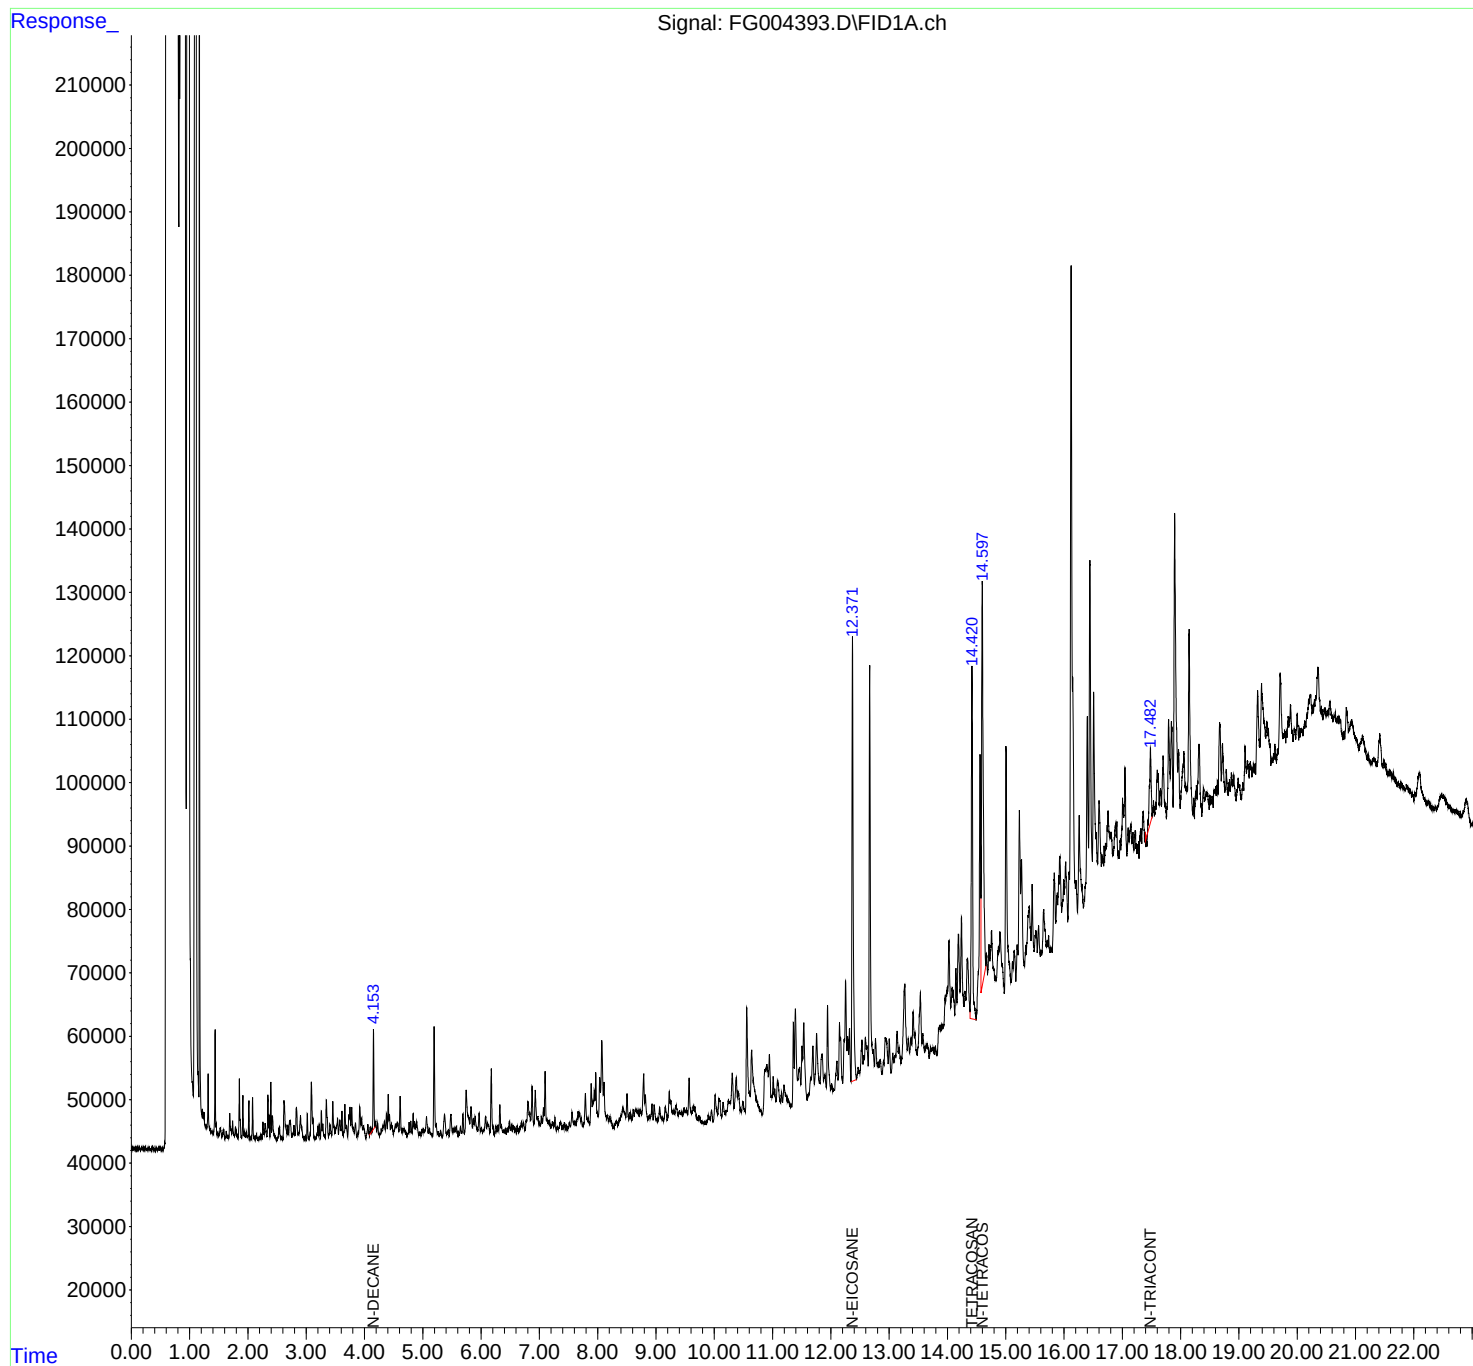


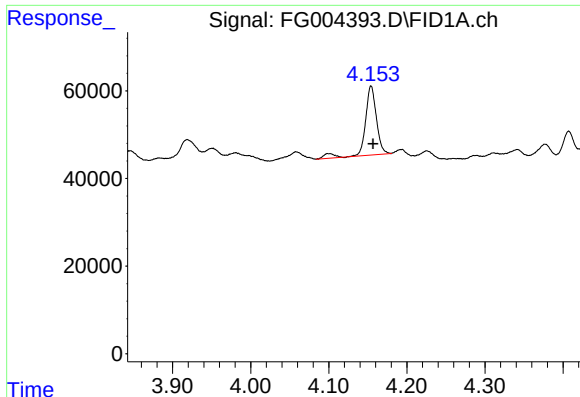

#2 N-DECANE


R.T.: 4.154 min
Delta R.T.: -0.002 min
Response: 158080
Conc: 1.50 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-21

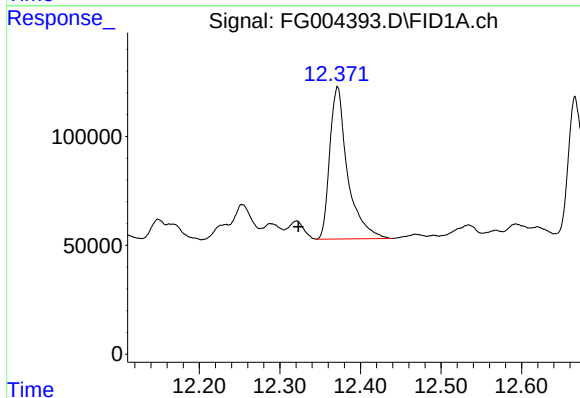


#7 N-EICOSANE

R.T.: 12.372 min
Delta R.T.: 0.049 min
Response: 1074181
Conc: 9.40 ug/ml

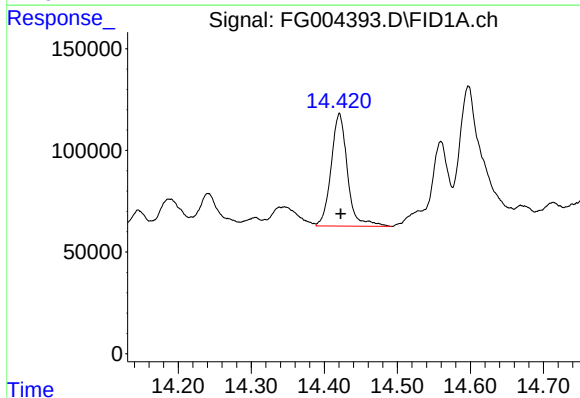


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.421 min
Delta R.T.: -0.002 min
Response: 860863
Conc: 8.35 ug/ml

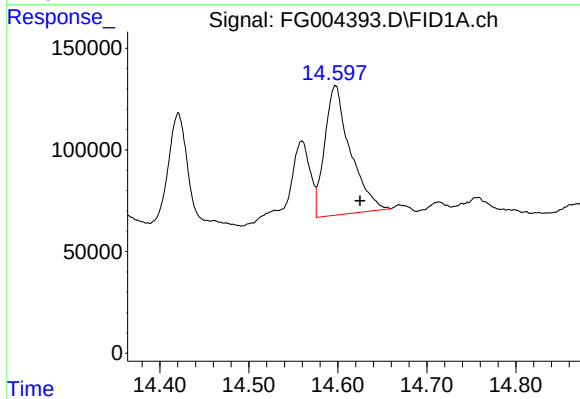

#10 N-TETRACOSANE

R.T.: 14.597 min
Delta R.T.: -0.028 min
Response: 1272576
Conc: 11.02 ug/ml

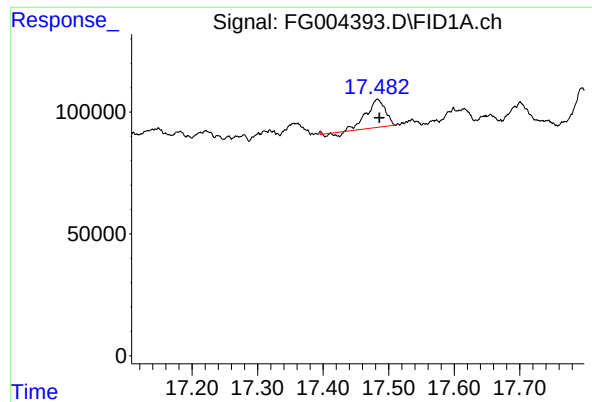

#13 N-TRIACONTANE

R.T.: 17.483 min
Delta R.T.: -0.003 min
Response: 221011
Conc: 1.86 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-21