

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032819\
 Data File : FG004395.D
 Signal(s) : FID1A.ch
 Acq On : 28 Mar 2019 13:14
 Operator : AJ\SJ
 Sample : K2090-02 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 P-5(0-10)

Integration File: autoint1.e
 Quant Time: Mar 29 03:43:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.421	898949	8.715 ug/ml
Target Compounds			
7) N-EICOSANE	12.369	2861189	25.029 ug/ml
8) N-DOCOSANE	13.536	294162	2.573 ug/ml
10) N-TETRACOSANE	14.596	1997318	17.290 ug/ml
12) N-OCTACOSANE	16.606	534648	4.621 ug/ml
13) N-TRIACONTANE	17.485	415168	3.500 ug/ml
14) N-DOTRIACONTANE	18.326	907587	7.740 ug/ml
16) N-HEXATRIACONTANE	19.886	1159286	10.400 ug/ml
18) N-TETRACONTANE	21.419	1537645	14.215 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032819\
Data File : FG004395.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2019 13:14
Operator : AJ\SJ
Sample : K2090-02 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :
P-5(0-10)

Integration File: autoint1.e
Quant Time: Mar 29 03:43:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

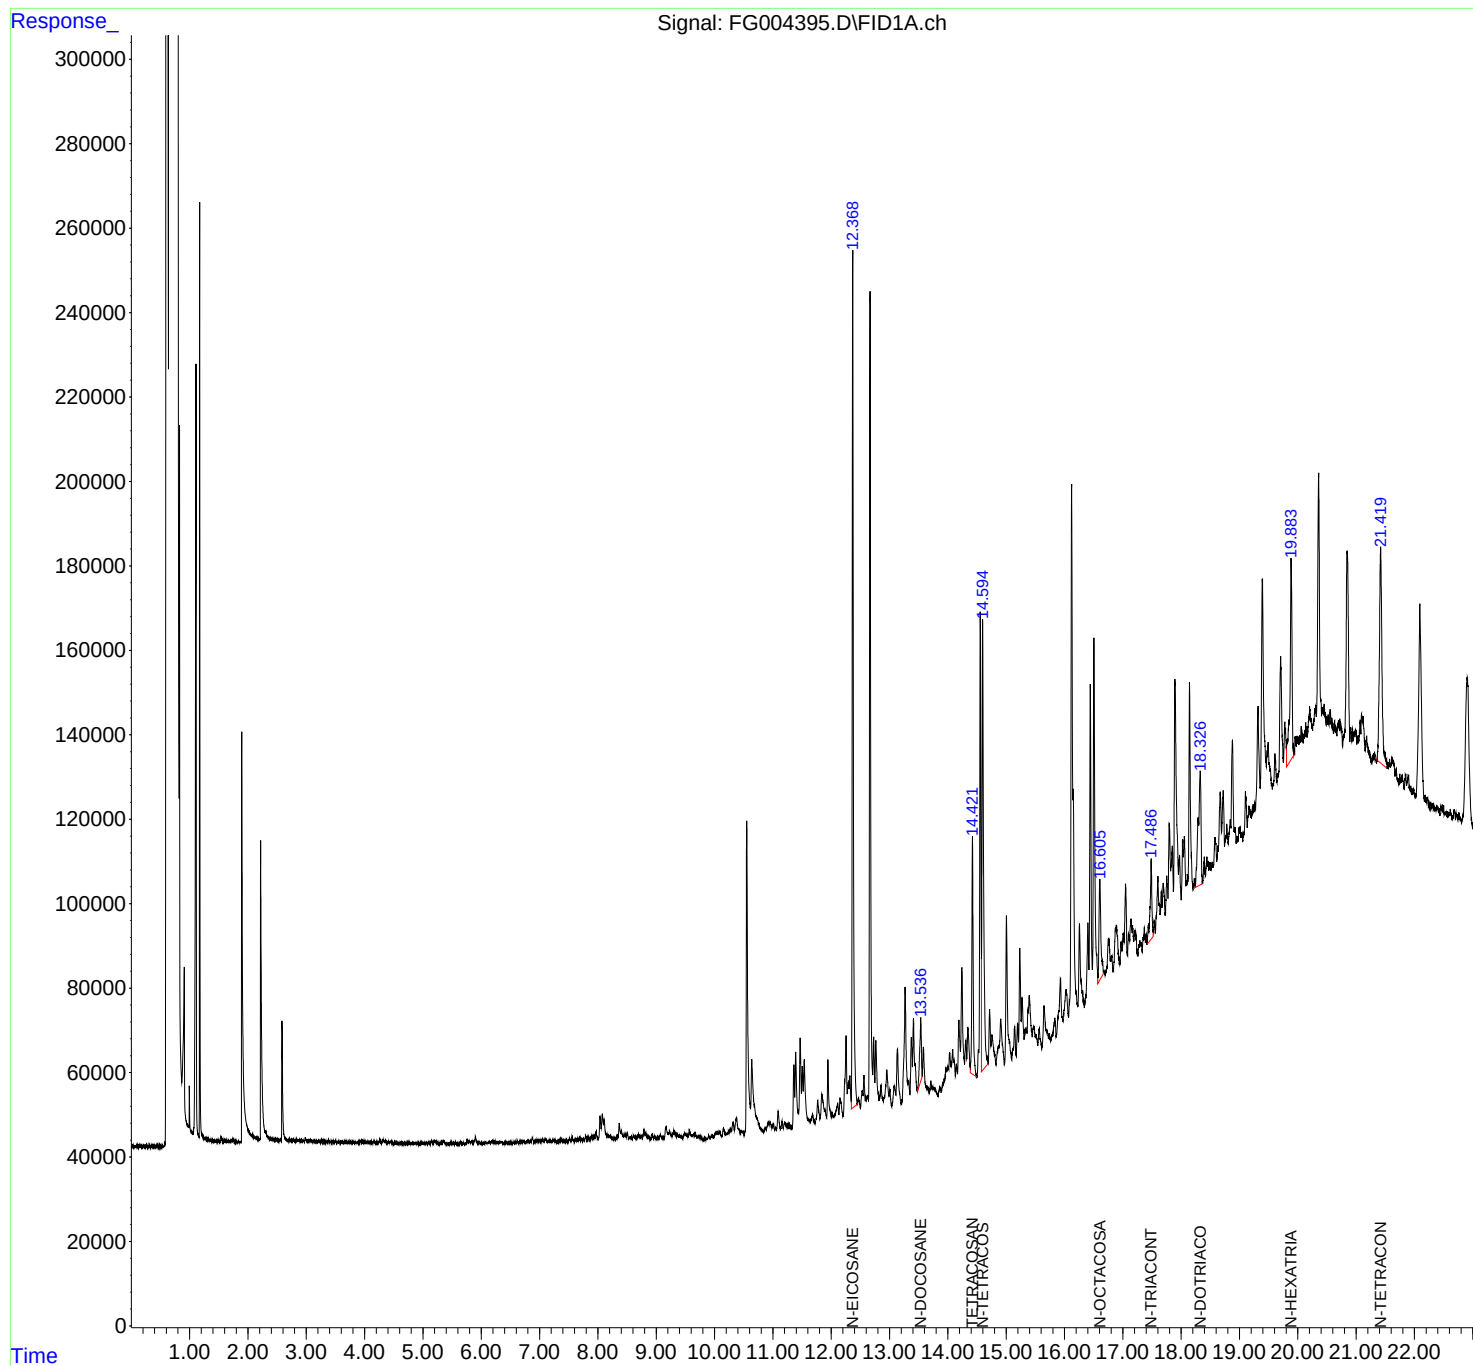


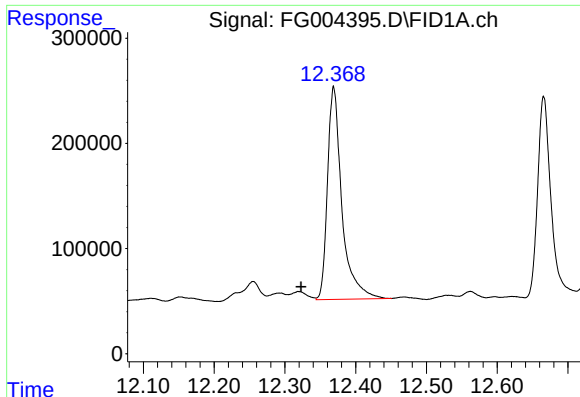

#7 N-EICOSANE


R.T.: 12.369 min
Delta R.T.: 0.046 min
Response: 2861189
Conc: 25.03 ug/ml

Instrument :
FID_G
ClientSampleId :
P-5(0-10)

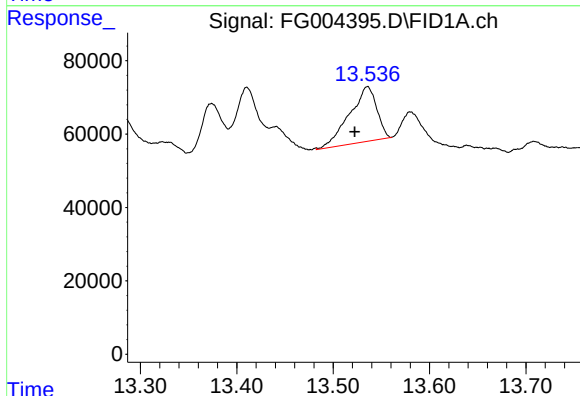


#8 N-DOCOSANE

R.T.: 13.536 min
Delta R.T.: 0.013 min
Response: 294162
Conc: 2.57 ug/ml

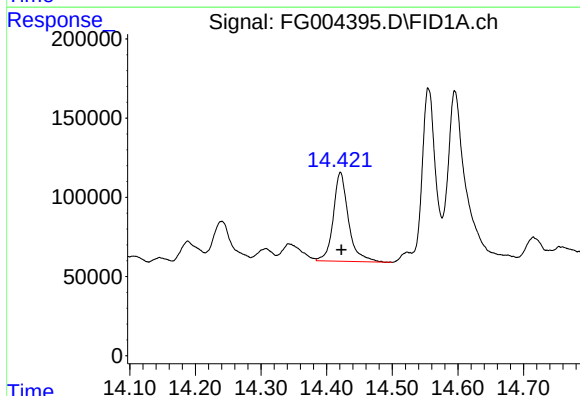


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.421 min
Delta R.T.: -0.001 min
Response: 898949
Conc: 8.72 ug/ml

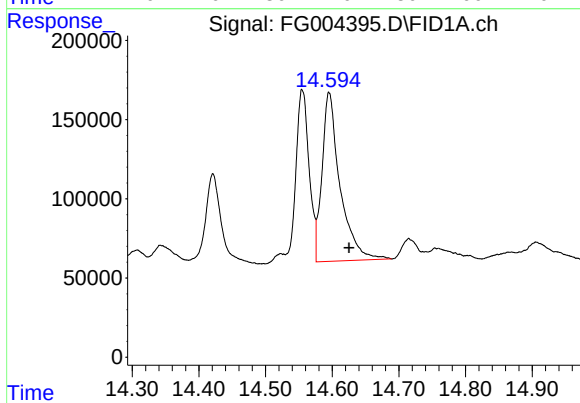

#10 N-TETRACOSANE


R.T.: 14.596 min
Delta R.T.: -0.029 min
Response: 1997318
Conc: 17.29 ug/ml

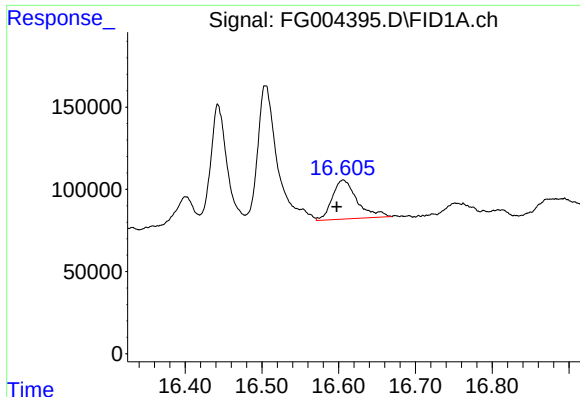

#12 N-OCTACOSANE


R.T.: 16.606 min
Delta R.T.: 0.009 min
Response: 534648
Conc: 4.62 ug/ml

Instrument :
FID_G
ClientSampleId :
P-5(0-10)

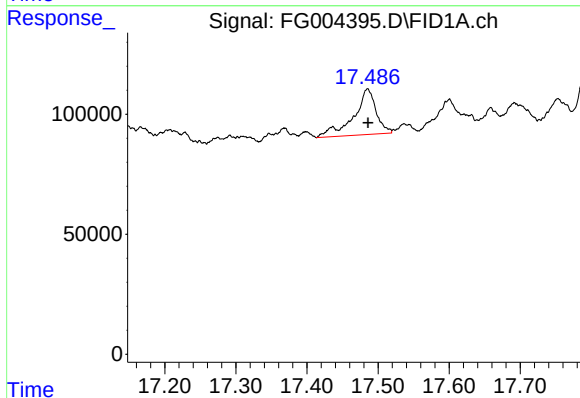


#13 N-TRIACONTANE

R.T.: 17.485 min
Delta R.T.: 0.000 min
Response: 415168
Conc: 3.50 ug/ml

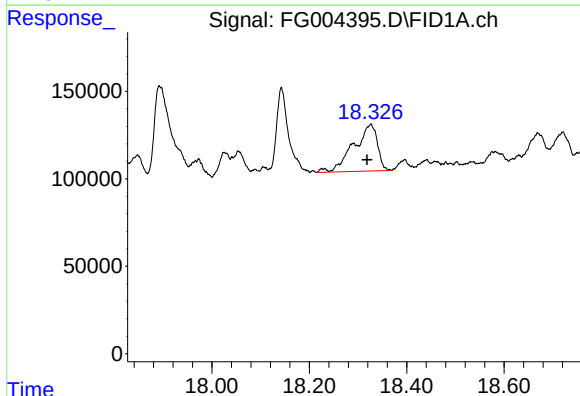


#14 N-DOTRIACONTANE

R.T.: 18.326 min
Delta R.T.: 0.007 min
Response: 907587
Conc: 7.74 ug/ml

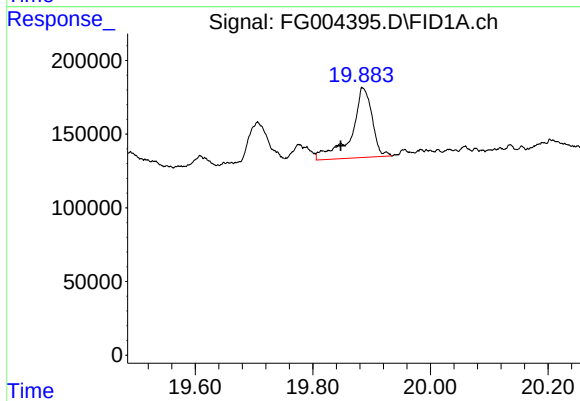

#16 N-HEXATRIACONTANE

R.T.: 19.886 min
Delta R.T.: 0.039 min
Response: 1159286
Conc: 10.40 ug/ml

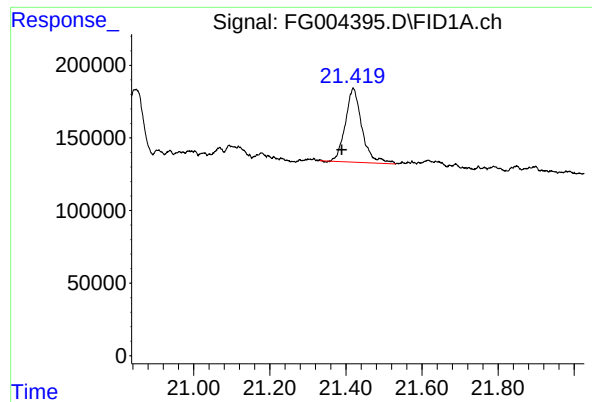

#18 N-TETRACONTANE

R.T.: 21.419 min
Delta R.T.: 0.031 min
Response: 1537645
Conc: 14.22 ug/ml

Instrument :
FID_G
ClientSampleId :
P-5(0-10)