

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032819\
Data File : FG004421.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2019 02:59
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 29 03:50:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.420	2039826	19.776 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.316	203418	1.735 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032819\
Data File : FG004421.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2019 02:59
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 29 03:50:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

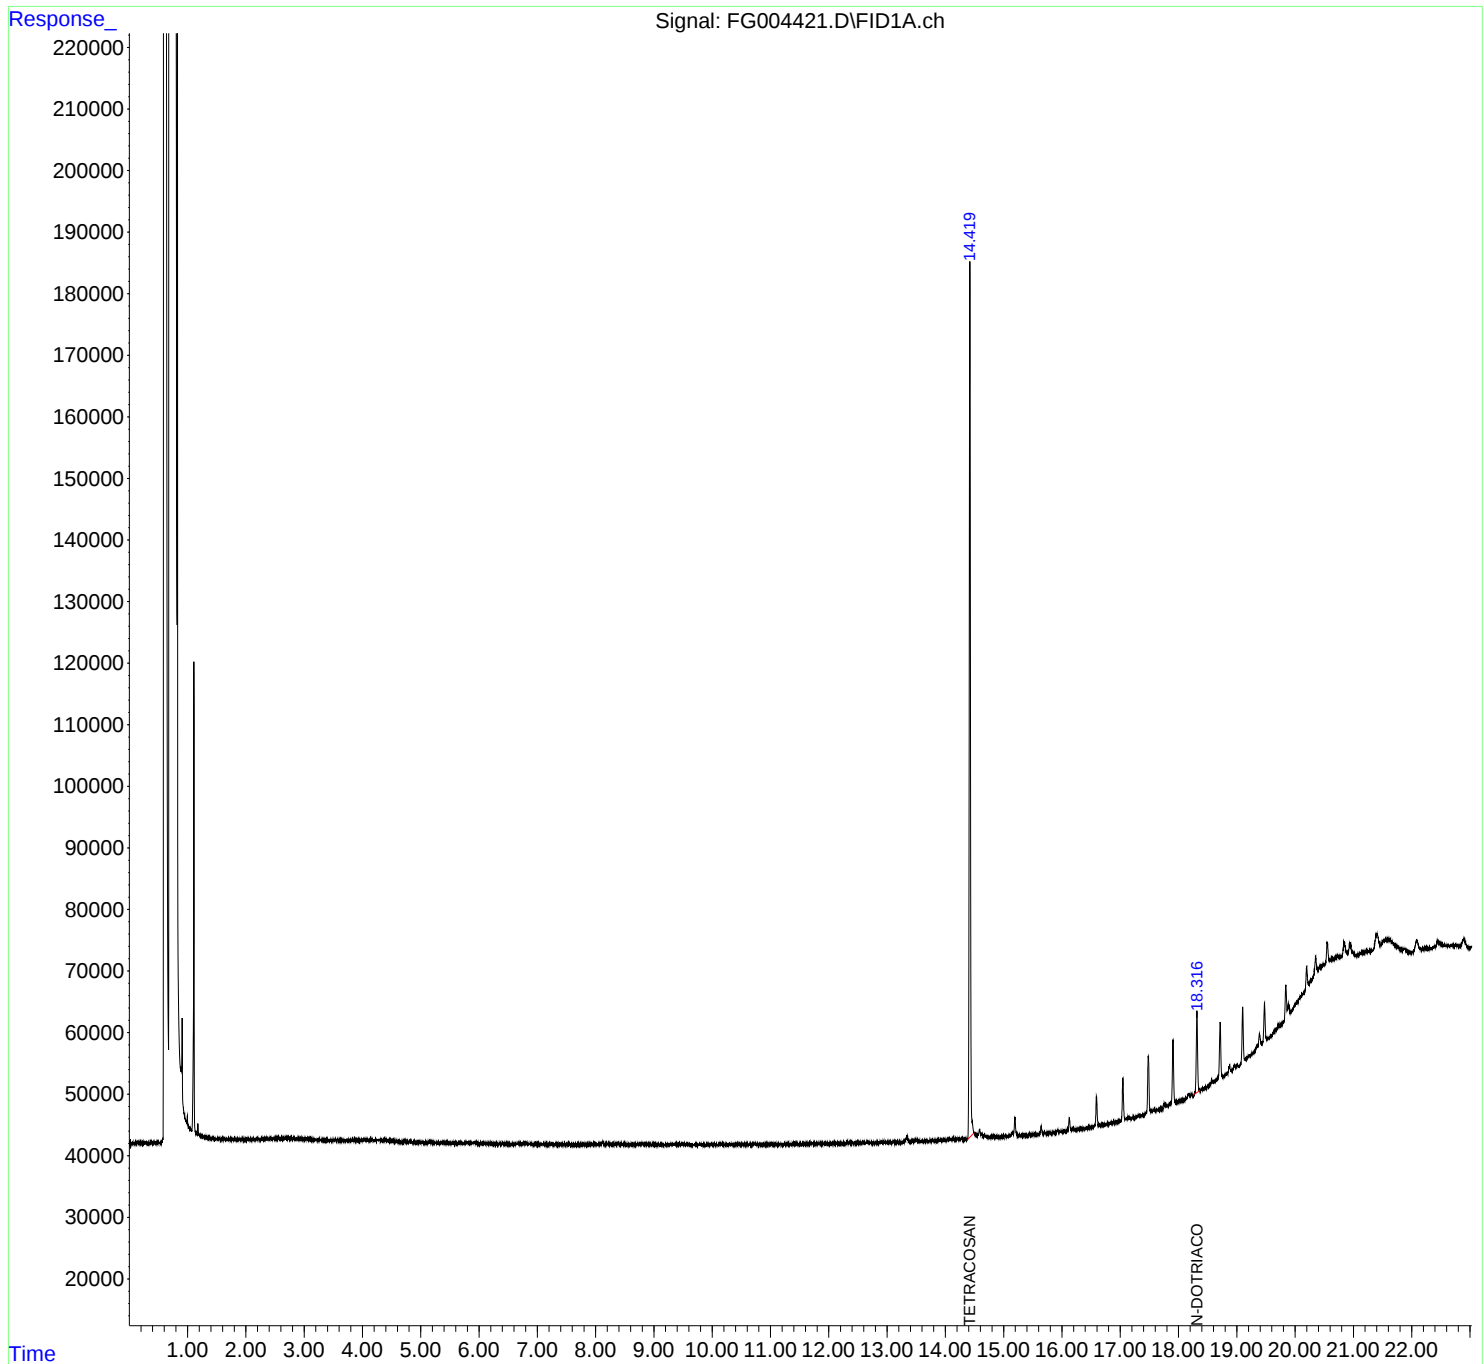


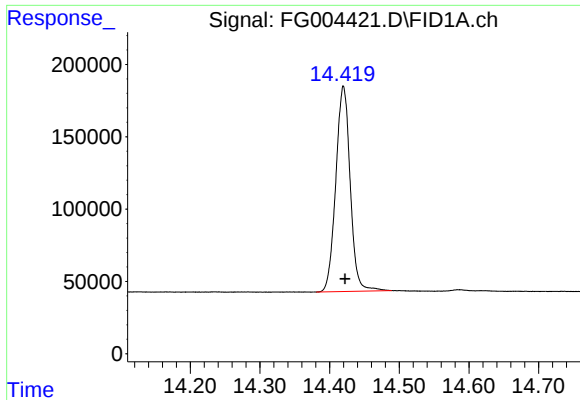

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.420 min
Delta R.T.: -0.003 min
Response: 2039826
Conc: 19.78 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

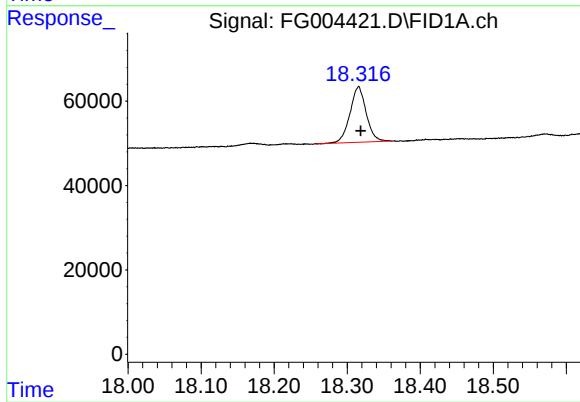

#14 N-DOTRIACONTANE

R.T.: 18.316 min
Delta R.T.: -0.003 min
Response: 203418
Conc: 1.73 ug/ml