

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032822\
Data File : FG009453.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2022 14:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:33:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	2353447	17.078 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.700	55911	0.392 ug/ml
14) N-DOTRIACONTANE	18.534	66040	0.497 ug/ml
15) N-TETRATRIACONTANE	19.322	112327	0.961 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032822\
Data File : FG009453.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2022 14:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:33:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

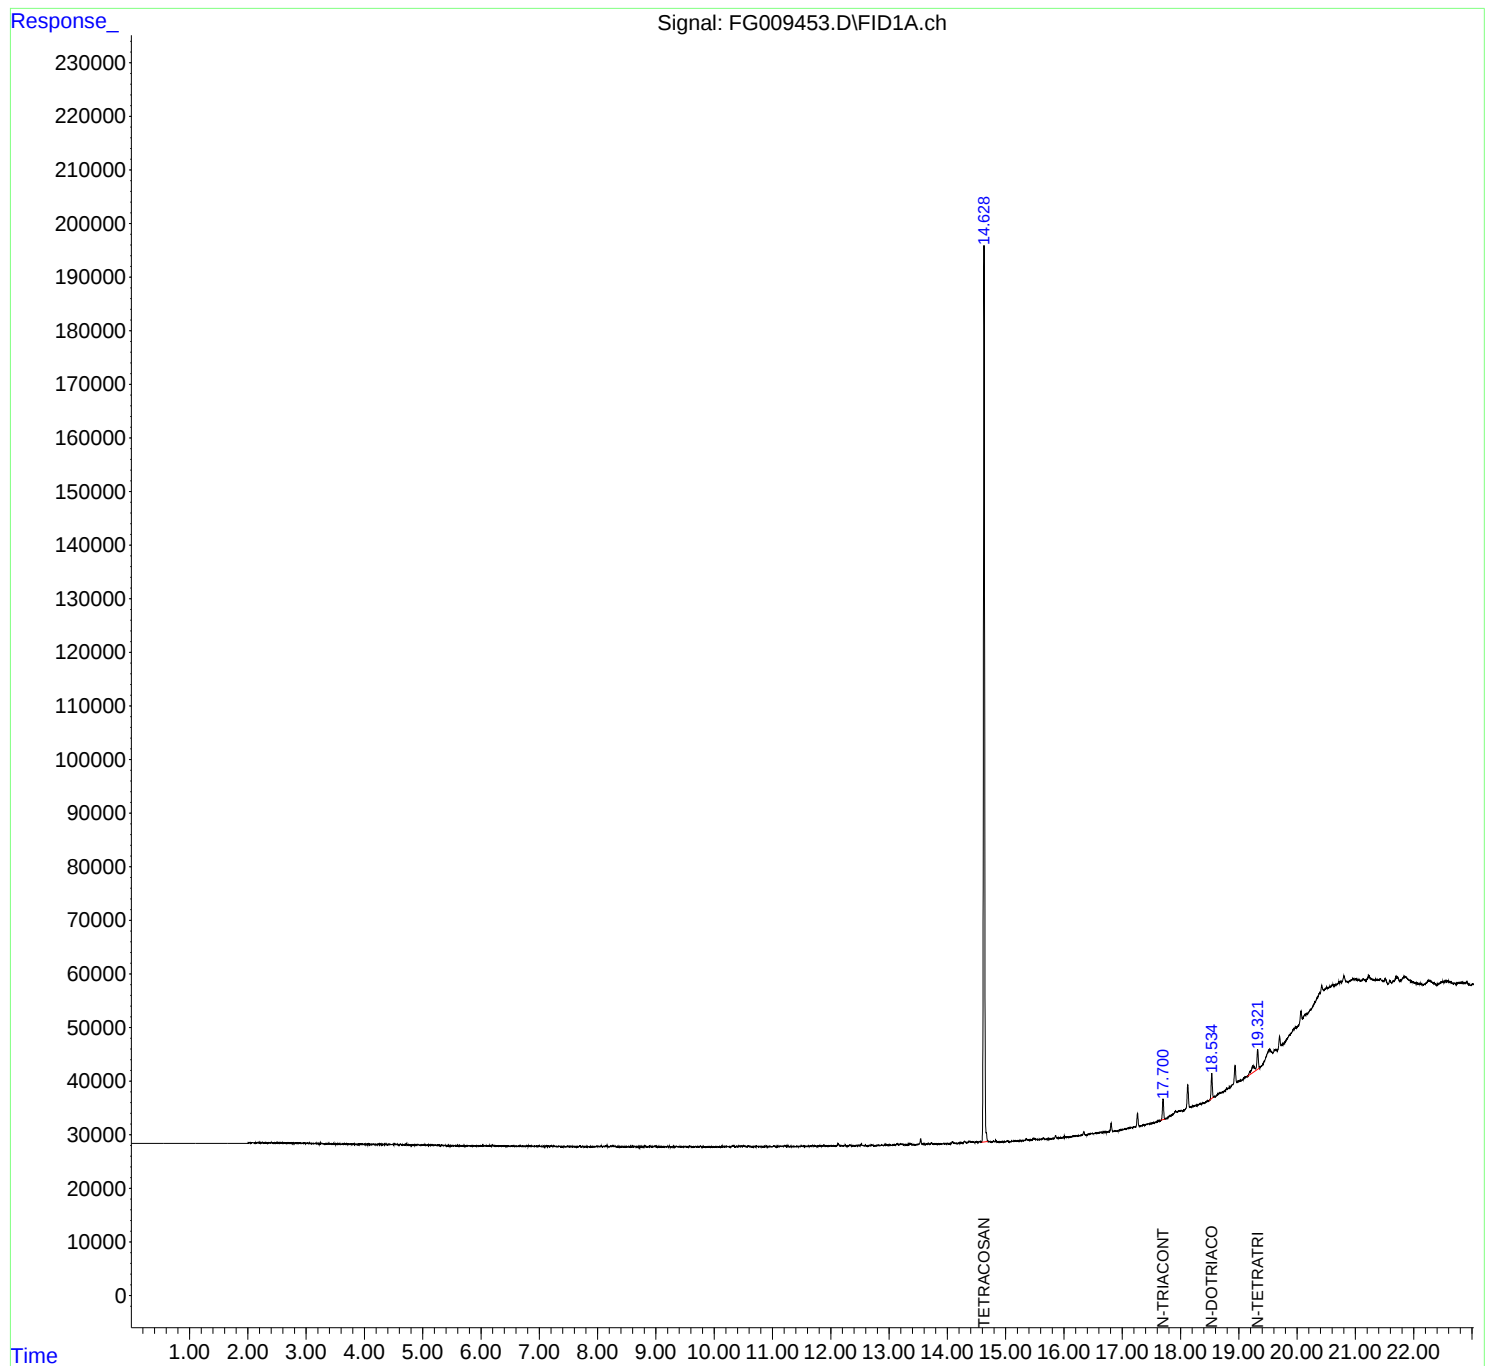


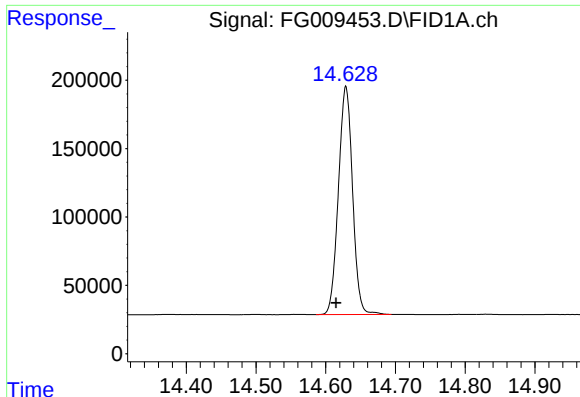

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.629 min
Delta R.T.: 0.014 min
Response: 2353447
Conc: 17.08 ug/ml

Instrument :
FID_G
ClientSampleId :

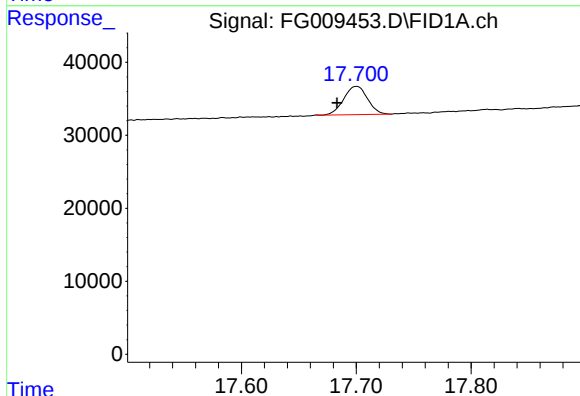


#13 N-TRIACONTANE

R.T.: 17.700 min
Delta R.T.: 0.017 min
Response: 55911
Conc: 0.39 ug/ml

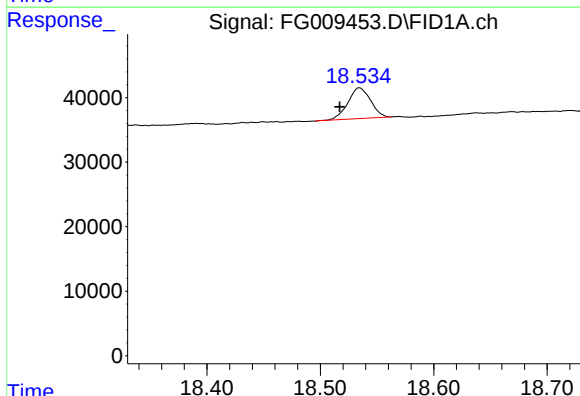

#14 N-DOTRIACONTANE

R.T.: 18.534 min
Delta R.T.: 0.018 min
Response: 66040
Conc: 0.50 ug/ml

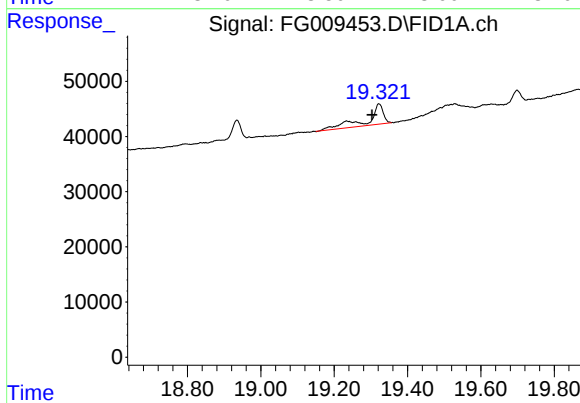

#15 N-TETRATRIACONTANE

R.T.: 19.322 min
Delta R.T.: 0.019 min
Response: 112327
Conc: 0.96 ug/ml