

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032822\
Data File : FG009447.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2022 11:30
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 29 02:32:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.357	3650077	24.476 ug/ml
12)	N-OCTACOSANE	16.812	3014038	20.338 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032822\
Data File : FG009447.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2022 11:30
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 29 02:32:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

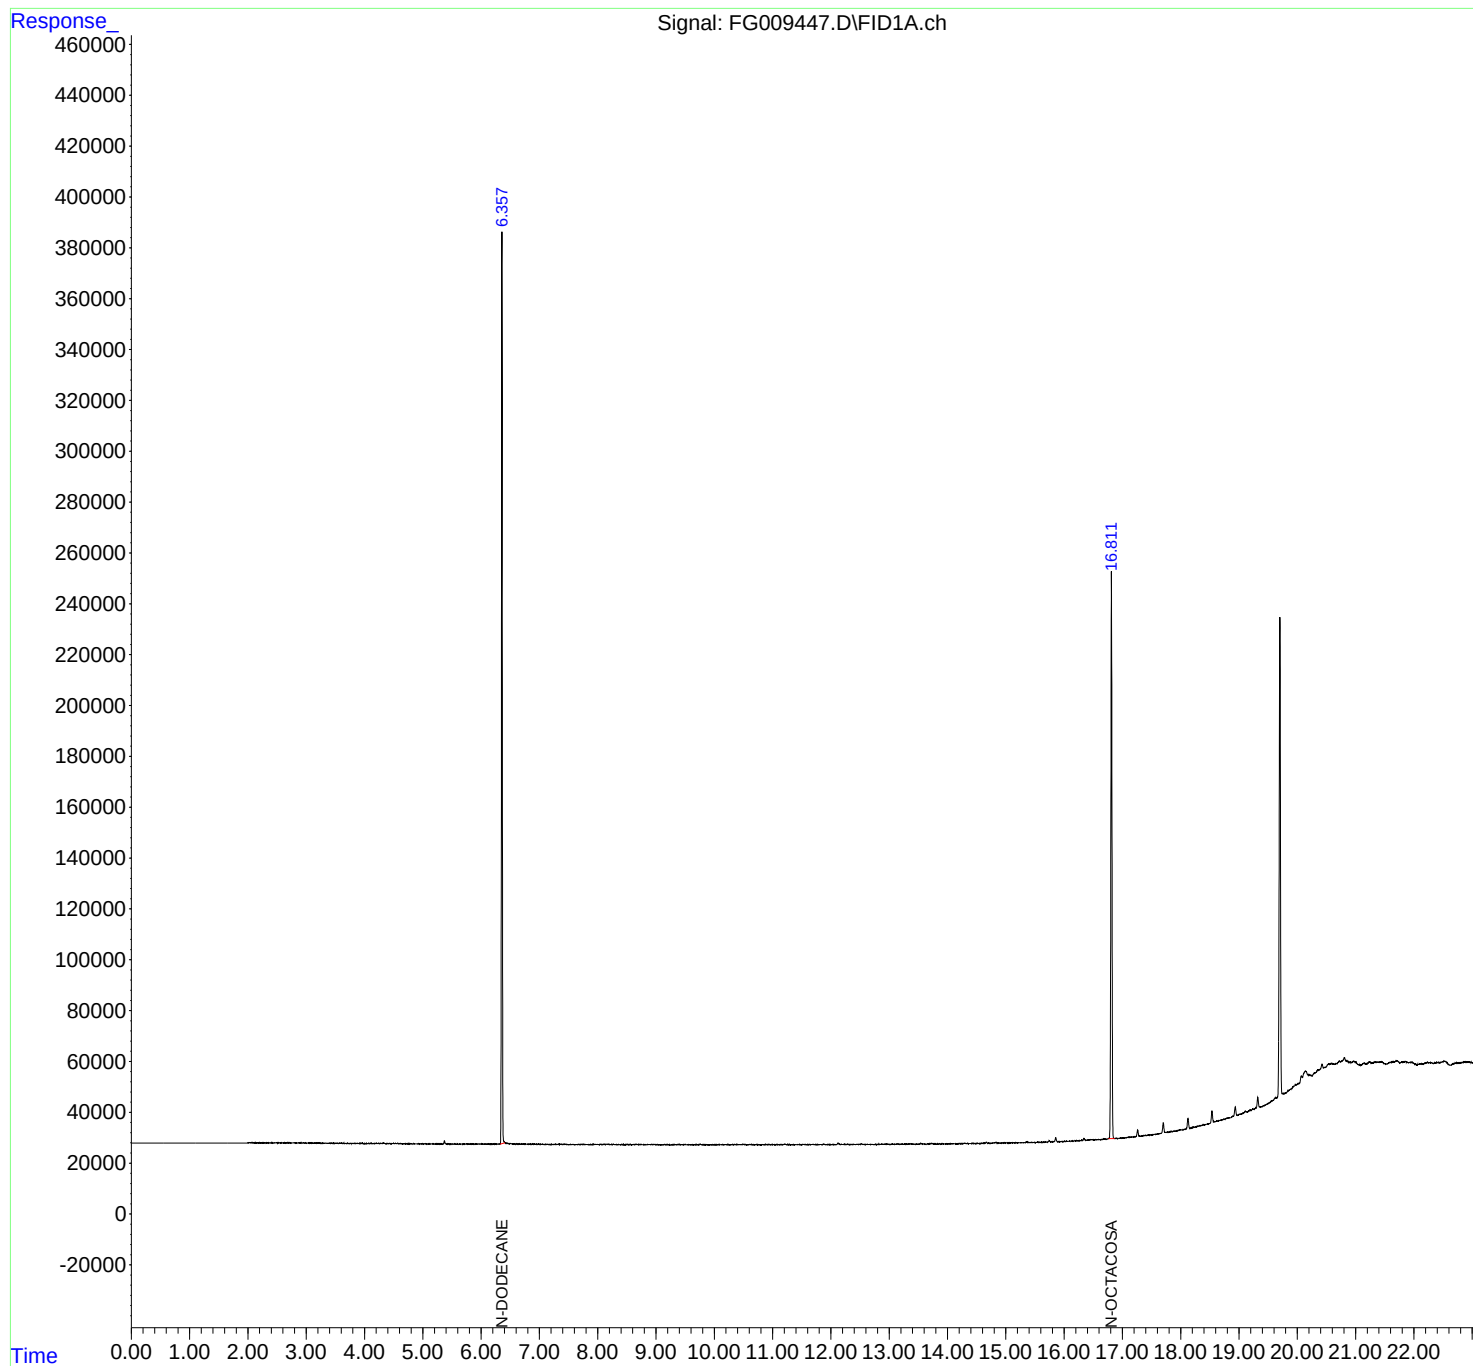


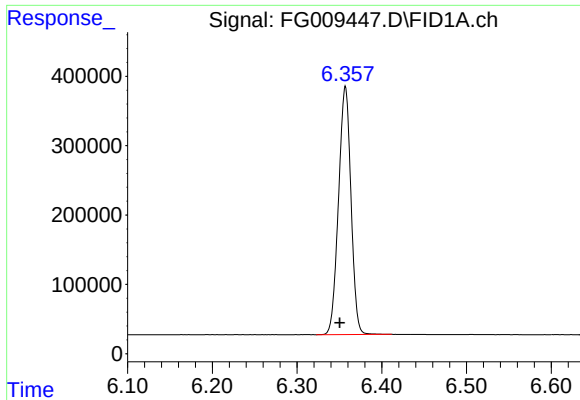

#3 N-DODECANE


R.T.: 6.357 min
Delta R.T.: 0.007 min
Response: 3650077
Conc: 24.48 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

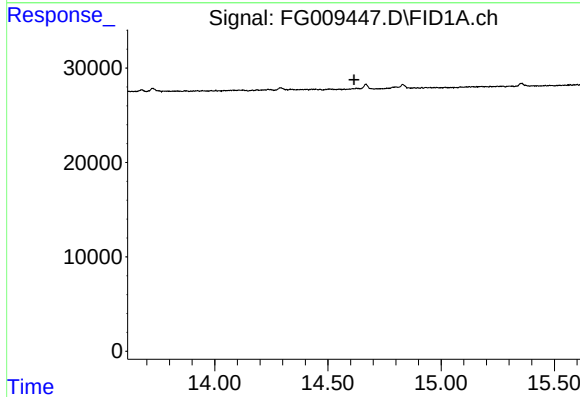

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.615 min
Response: 0
Conc: N.D.

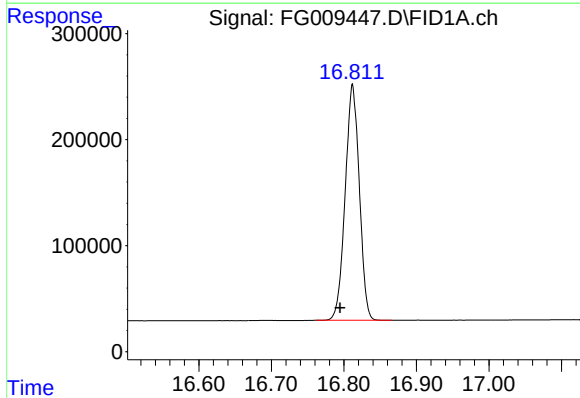

#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: 0.017 min
Response: 3014038
Conc: 20.34 ug/ml