

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004463.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2019 01:19
Operator : AJ\SJ
Sample : K2121-08 25X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DUP

Integration File: autoint1.e
Quant Time: Mar 30 04:22:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.151	1432387	13.570 ug/ml
3) N-DODECANE	6.172	288689	2.740 ug/ml
4) N-TETRADECANE	7.964	298799	2.758 ug/ml
5) N-HEXADECANE	9.564	107834	0.964 ug/ml
6) N-OCTADECANE	11.003	309579	2.729 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004463.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2019 01:19
Operator : AJ\SJ
Sample : K2121-08 25X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DUP

Integration File: autoint1.e
Quant Time: Mar 30 04:22:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

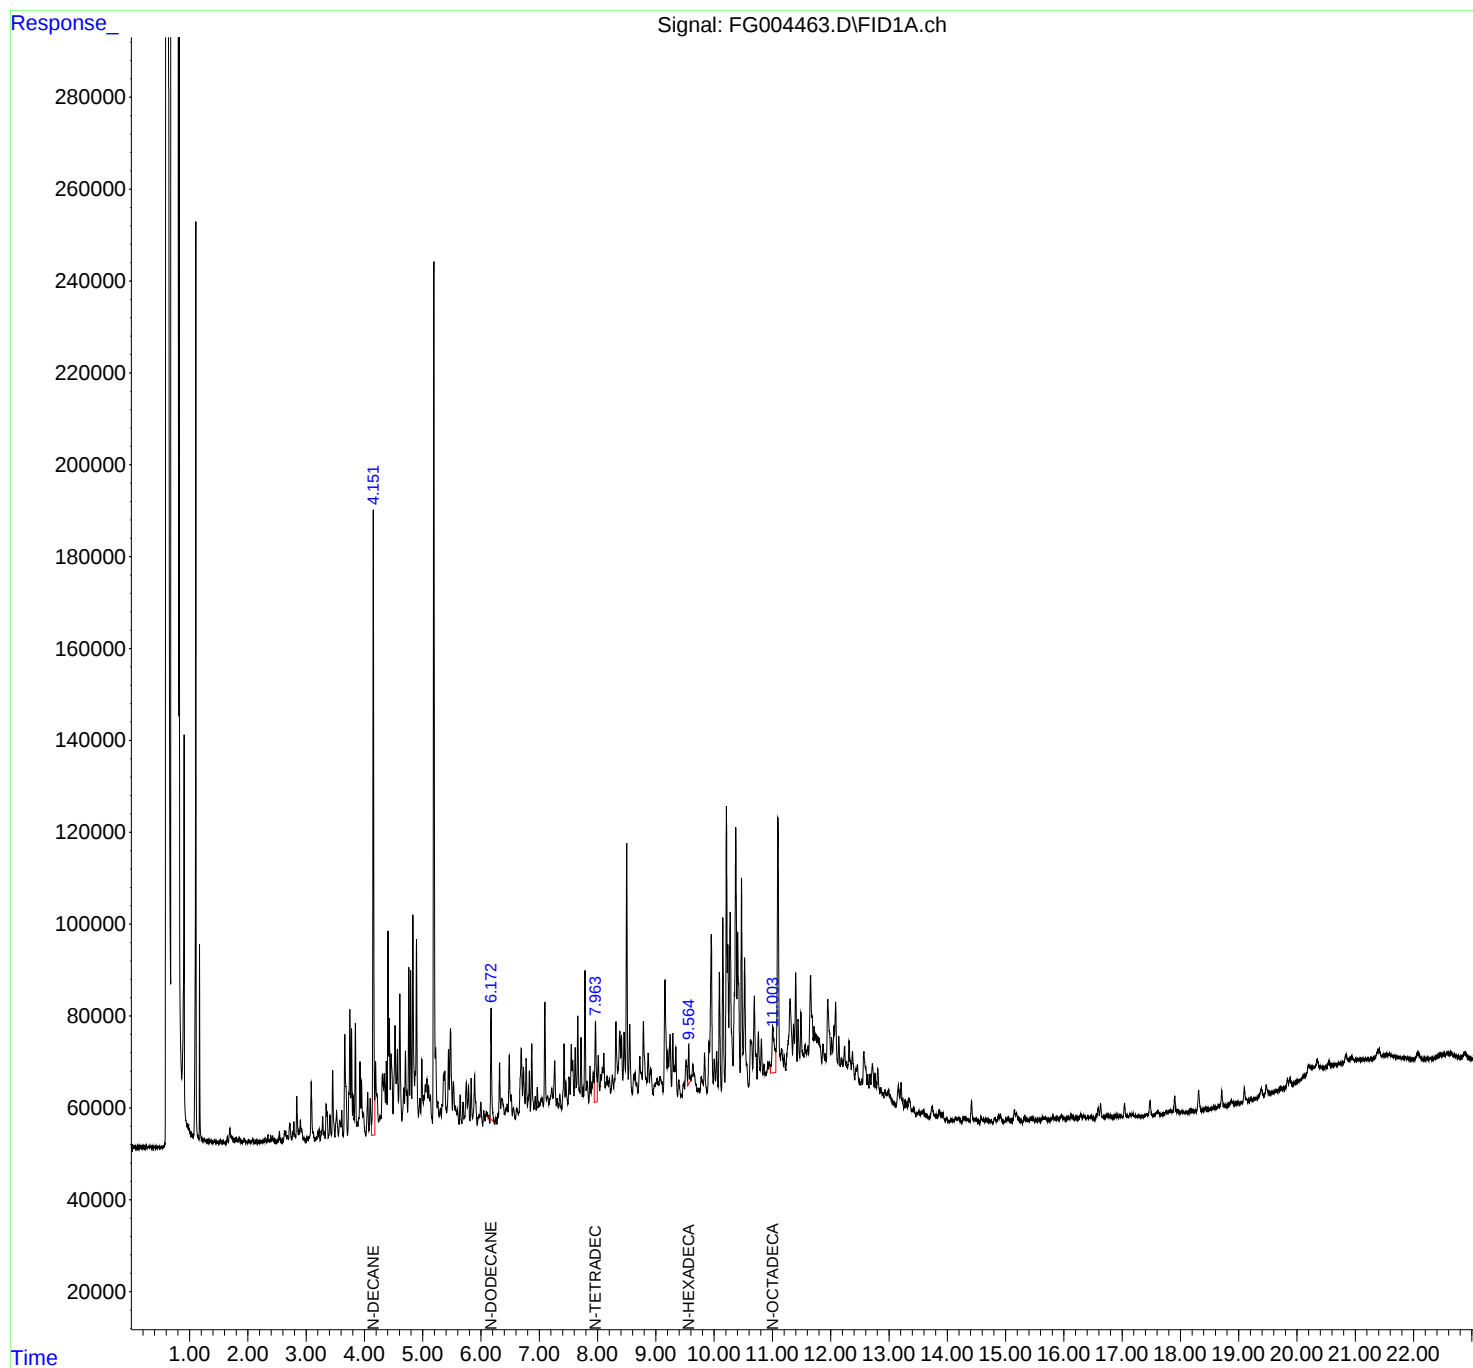


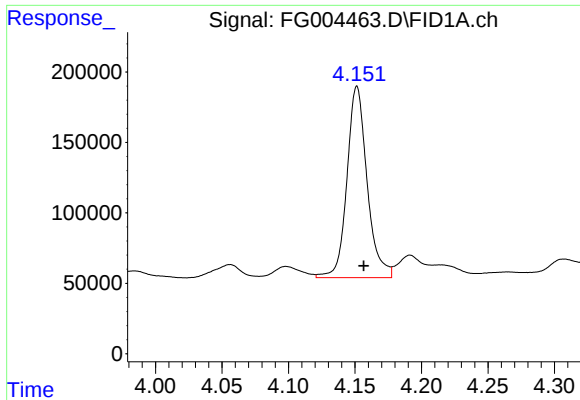

#2 N-DECANE


R.T.: 4.151 min
Delta R.T.: -0.005 min
Response: 1432387
Conc: 13.57 ug/ml

Instrument :
FID_G
ClientSampleId :
DUP

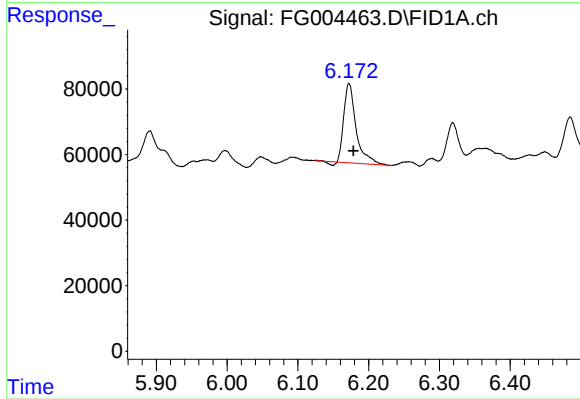


#3 N-DODECANE

R.T.: 6.172 min
Delta R.T.: -0.006 min
Response: 288689
Conc: 2.74 ug/ml

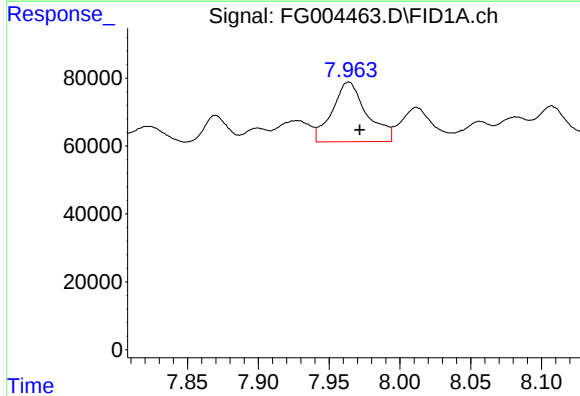


#4 N-TETRADECANE

R.T.: 7.964 min
Delta R.T.: -0.008 min
Response: 298799
Conc: 2.76 ug/ml

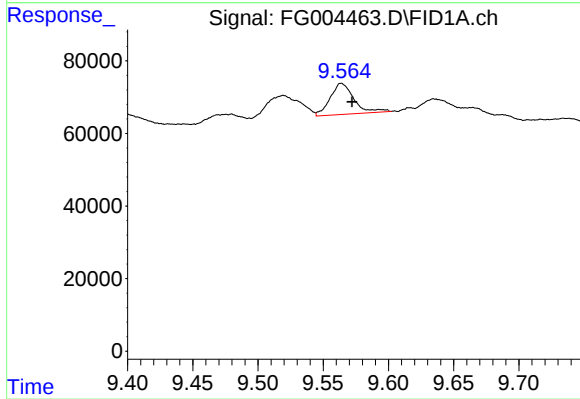

#5 N-HEXADECANE


R.T.: 9.564 min
Delta R.T.: -0.008 min
Response: 107834
Conc: 0.96 ug/ml

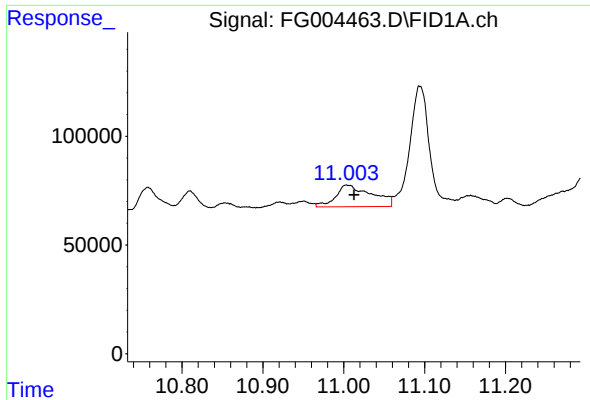

#6 N-OCTADECANE

R.T.: 11.003 min
Delta R.T.: -0.010 min
Response: 309579
Conc: 2.73 ug/ml

Instrument :
FID_G
ClientSampleId :
DUP

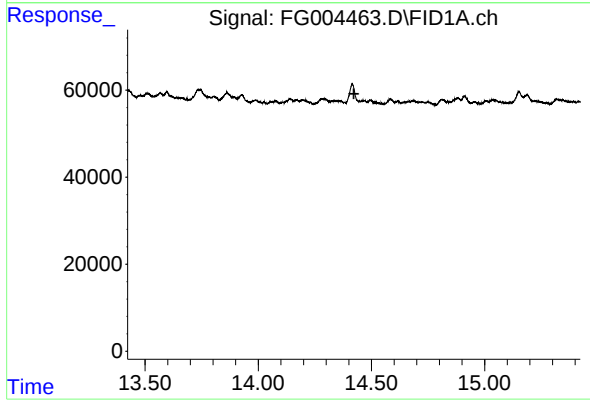

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.