

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
 Data File : FG004468.D
 Signal(s) : FID1A.ch
 Acq On : 30 Mar 2019 04:22
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 30 06:03:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.172	2927191	27.783 ug/ml
12)	N-OCTACOSANE	16.590	3499371	30.248 ug/ml
13)	N-TRIACONTANE	17.477	390400	3.291 ug/ml
14)	N-DOTRIACONTANE	18.310	512478	4.370 ug/ml
15)	N-TETRATRIACONTANE	19.092	392584	3.523 ug/ml
16)	N-HEXATRIACONTANE	19.835	165611	1.486 ug/ml
17)	N-OCTATRIACONTANE	20.544	154036	1.550 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004468.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2019 04:22
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 30 06:03:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

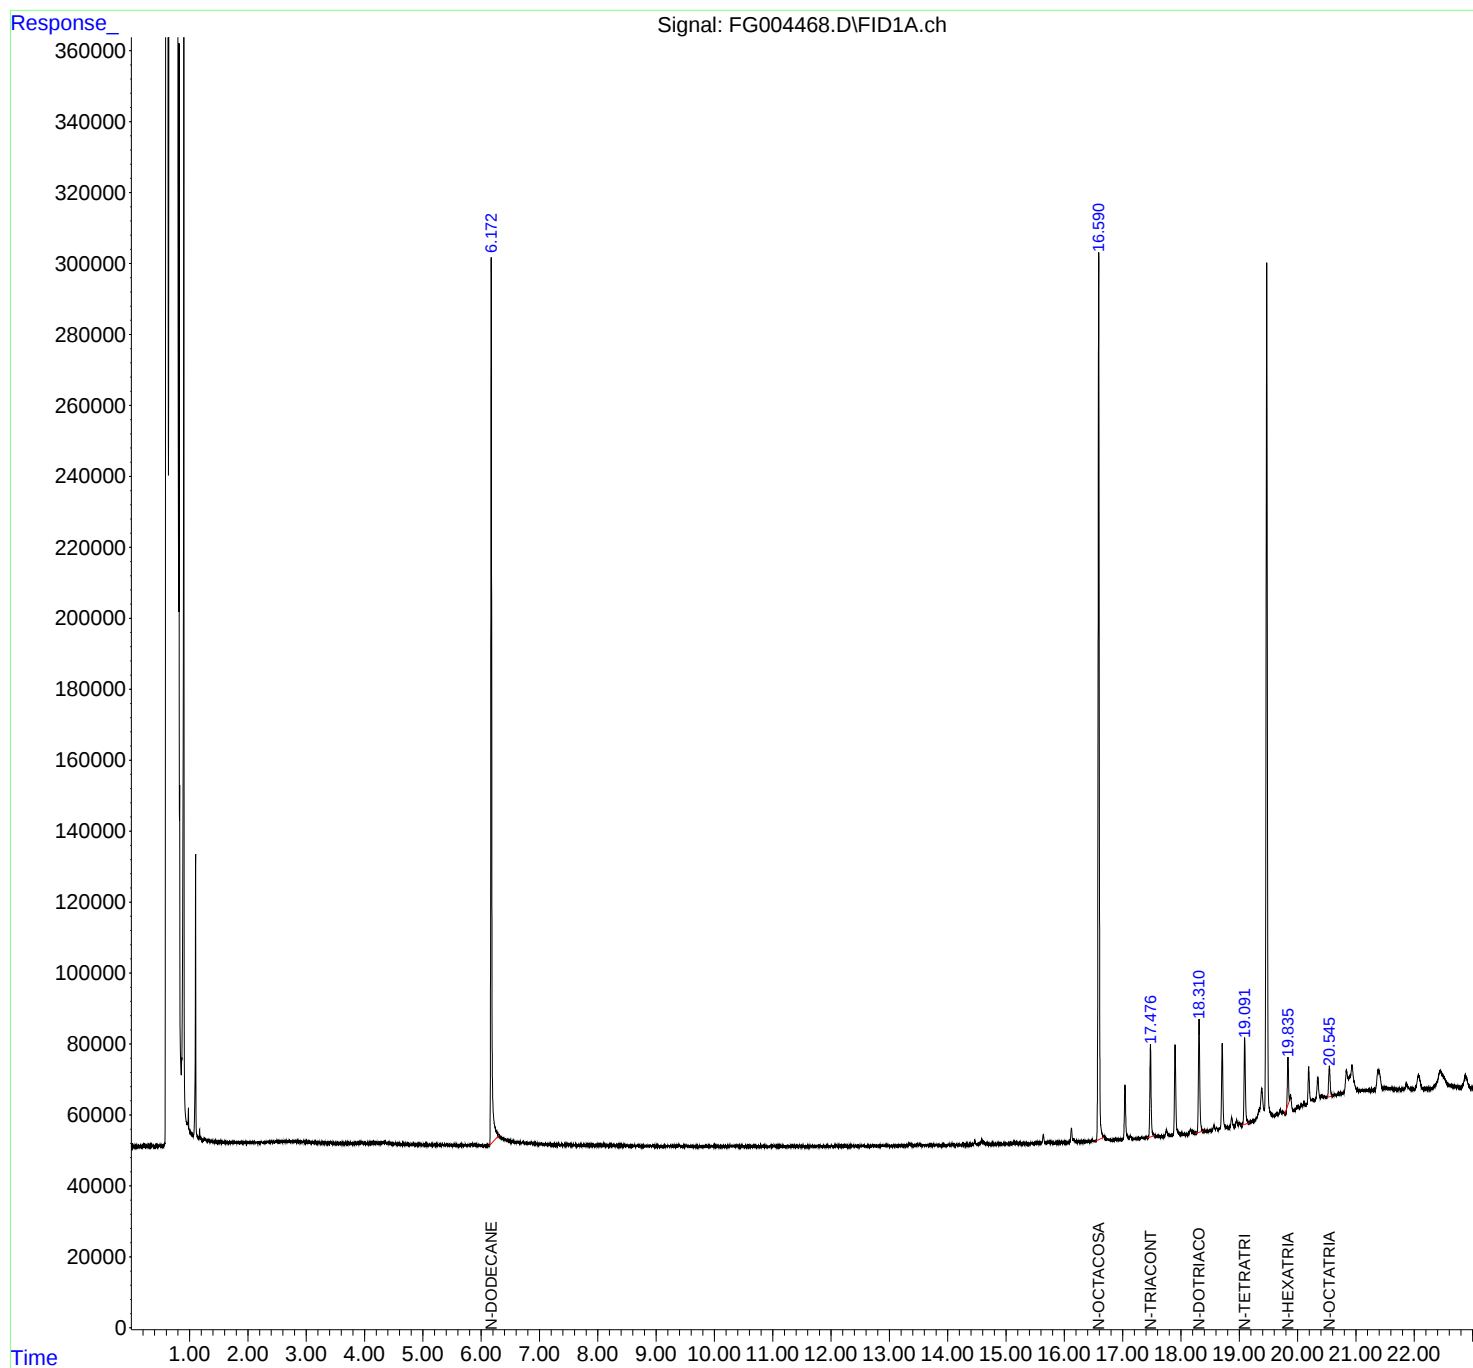


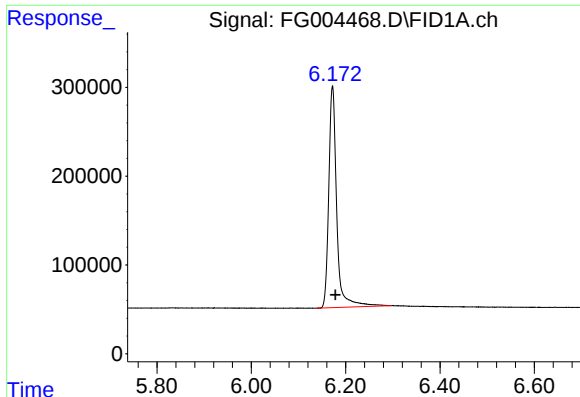

#3 N-DODECANE


R.T.: 6.172 min
Delta R.T.: -0.006 min
Response: 2927191
Conc: 27.78 ug/ml

Instrument :
FID_G
ClientSampleId :

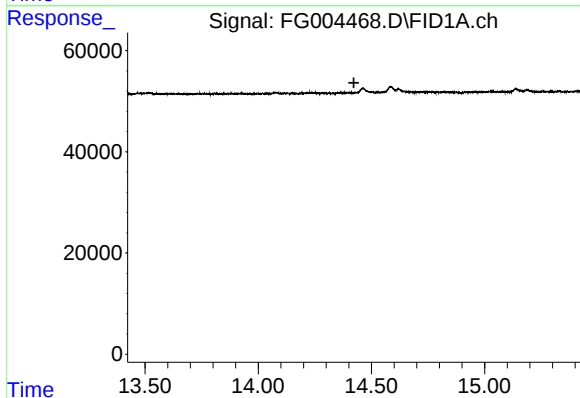


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

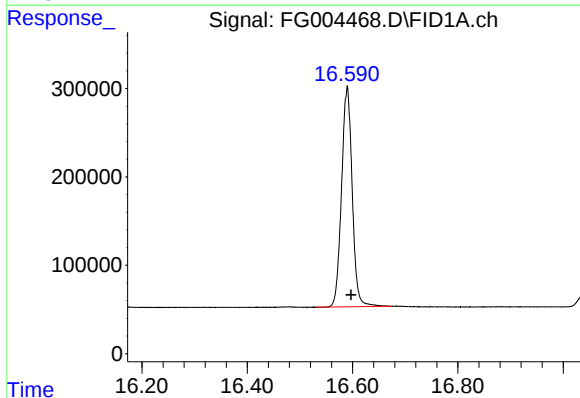


#12 N-OCTACOSANE

R.T.: 16.590 min
Delta R.T.: -0.007 min
Response: 3499371
Conc: 30.25 ug/ml

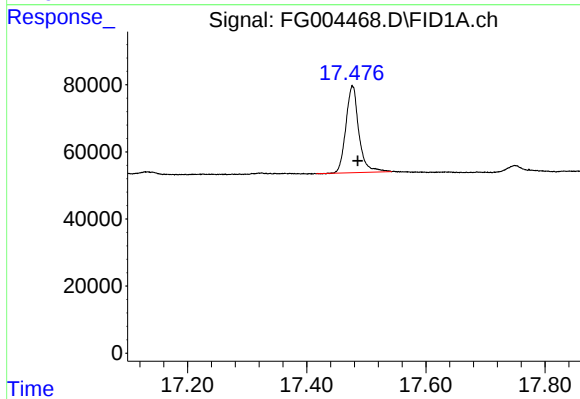

#13 N-TRIACONTANE


R.T.: 17.477 min
Delta R.T.: -0.009 min
Response: 390400
Conc: 3.29 ug/ml

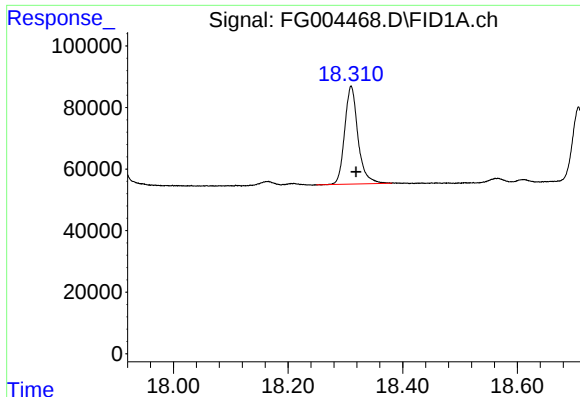

#14 N-DOTRIACONTANE


R.T.: 18.310 min
Delta R.T.: -0.008 min
Response: 512478
Conc: 4.37 ug/ml

Instrument :
FID_G
ClientSampleId :

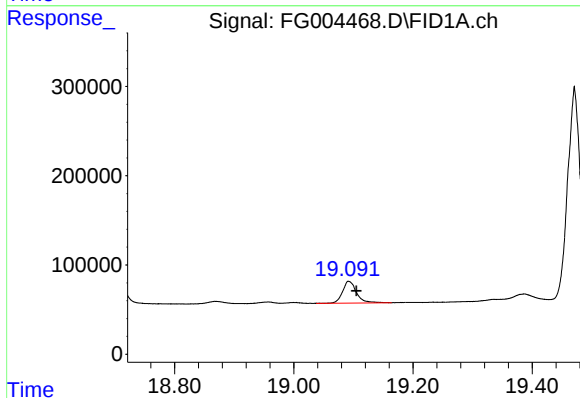


#15 N-TETRATRIACONTANE

R.T.: 19.092 min
Delta R.T.: -0.013 min
Response: 392584
Conc: 3.52 ug/ml

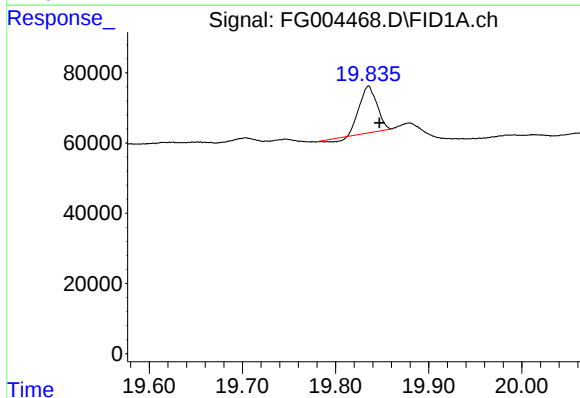

#16 N-HEXATRIACONTANE

R.T.: 19.835 min
Delta R.T.: -0.012 min
Response: 165611
Conc: 1.49 ug/ml

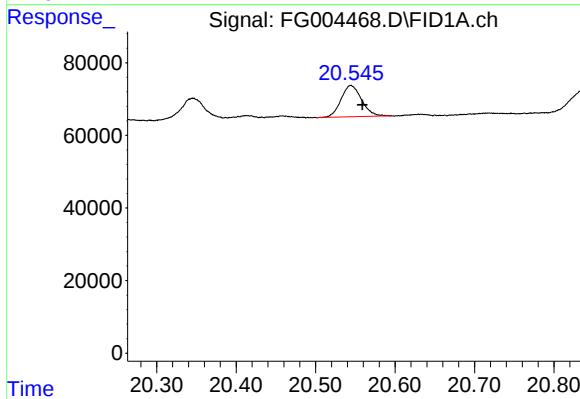

#17 N-OCTATRIACONTANE

R.T.: 20.544 min
Delta R.T.: -0.015 min
Response: 154036
Conc: 1.55 ug/ml