

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
 Data File : FG004471.D
 Signal(s) : FID1A.ch
 Acq On : 30 Mar 2019 05:54
 Operator : AJ\SJ
 Sample : K2115-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 01 01:49:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.414	1718198	16.658 ug/ml
Target Compounds			
2) N-DECANE	4.194	8180893	77.503 ug/ml
3) N-DODECANE	6.167	1602359	15.209 ug/ml
4) N-TETRADECANE	7.959	3890465	35.907 ug/ml
5) N-HEXADECANE	9.572	8501623	75.988 ug/ml
6) N-OCTADECANE	11.018	3134216	27.632 ug/ml
7) N-EICOSANE	12.316	862720	7.547 ug/ml
8) N-DOCOSANE	13.527	151786	1.328 ug/ml
10) N-TETRACOSANE	14.632	214727	1.859 ug/ml
13) N-TRIACONTANE	17.475	106415	0.897 ug/ml
14) N-DOTRIACONTANE	18.306	135938	1.159 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004471.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2019 05:54
Operator : AJ\SJ
Sample : K2115-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 01:49:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

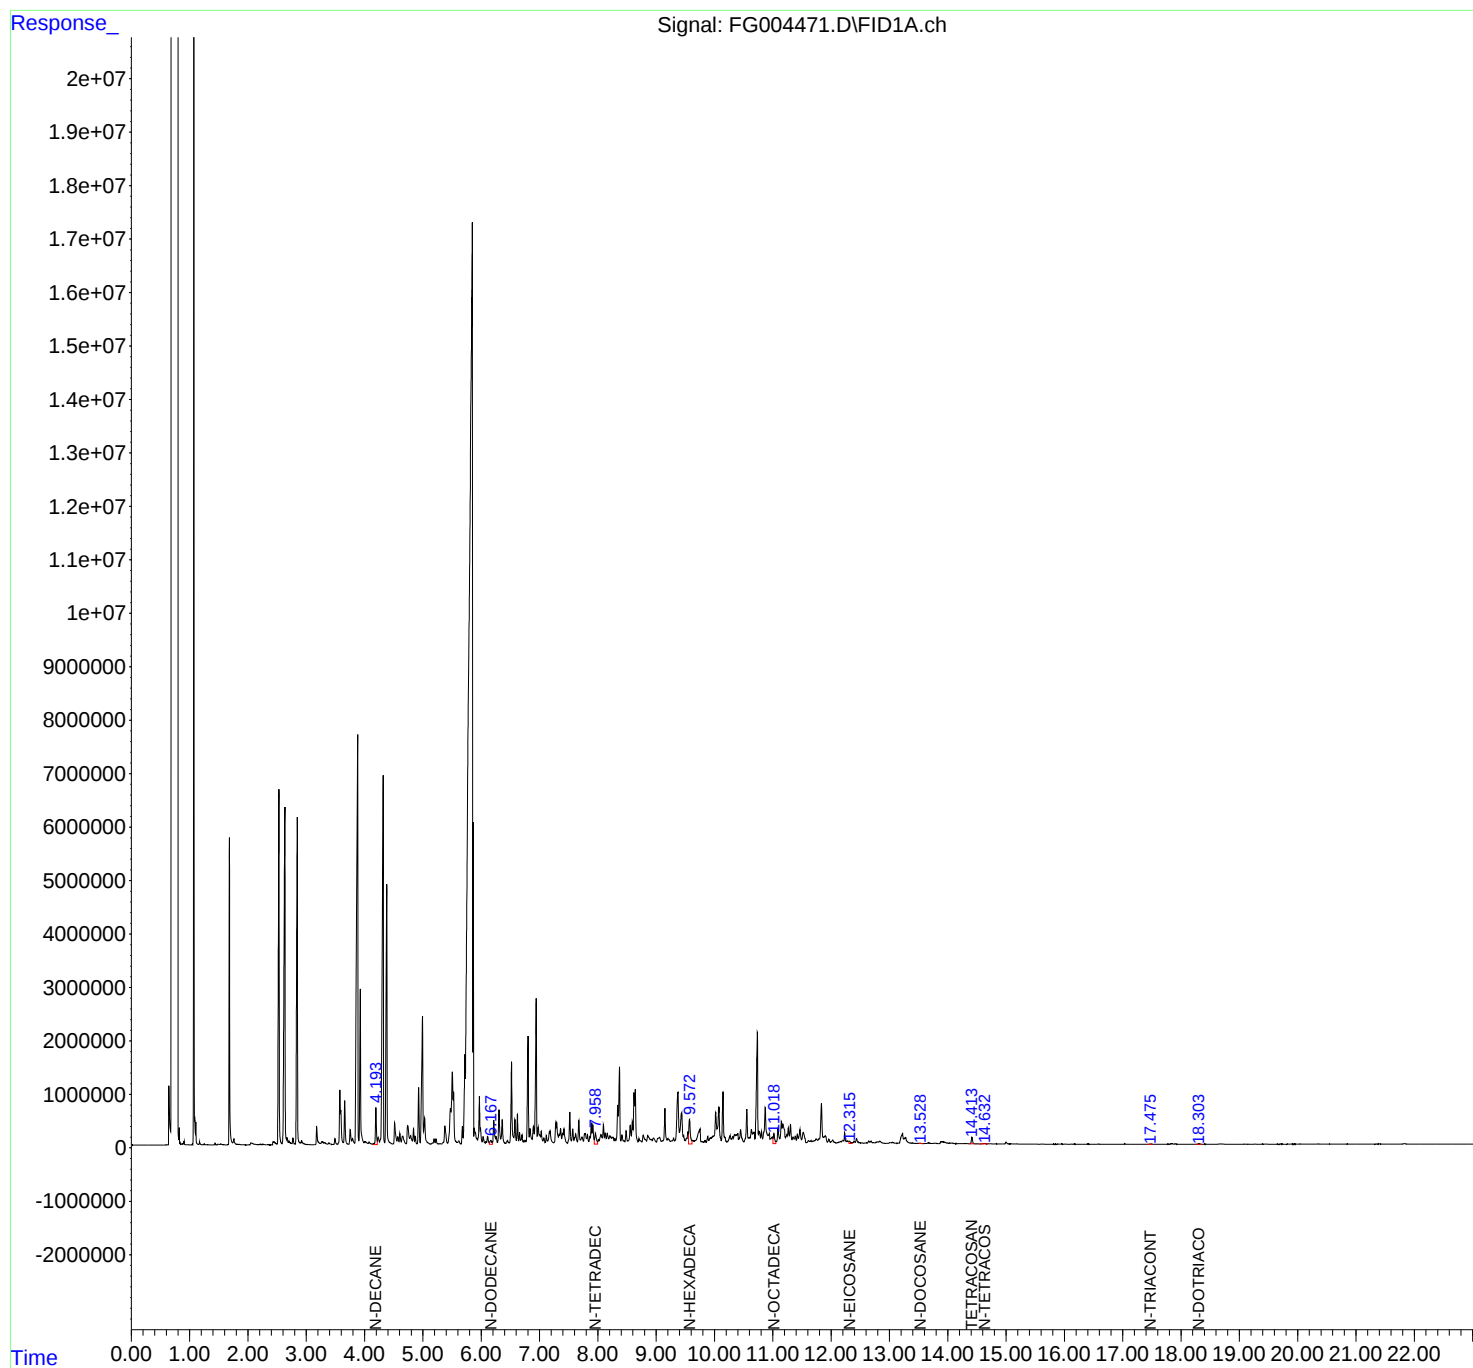


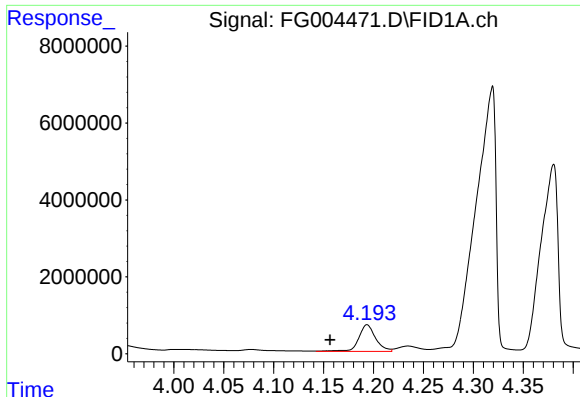

#2 N-DECANE


R.T.: 4.194 min
Delta R.T.: 0.037 min
Response: 8180893
Conc: 77.50 ug/ml

Instrument :
FID_G
ClientSampleId :

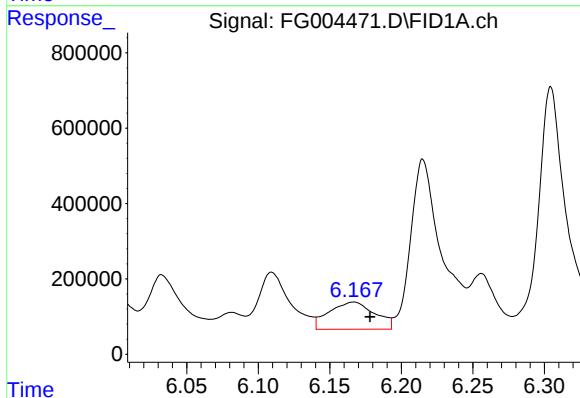


#3 N-DODECANE

R.T.: 6.167 min
Delta R.T.: -0.011 min
Response: 1602359
Conc: 15.21 ug/ml

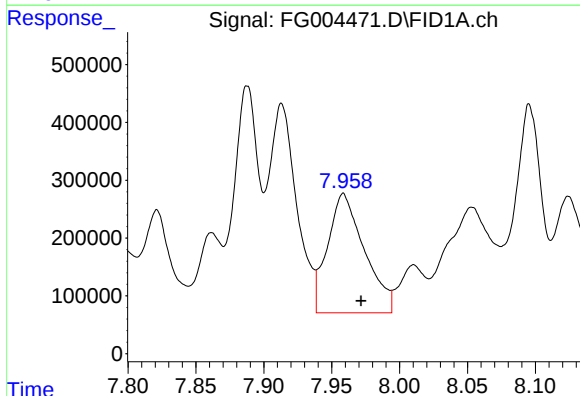


#4 N-TETRADECANE

R.T.: 7.959 min
Delta R.T.: -0.013 min
Response: 3890465
Conc: 35.91 ug/ml

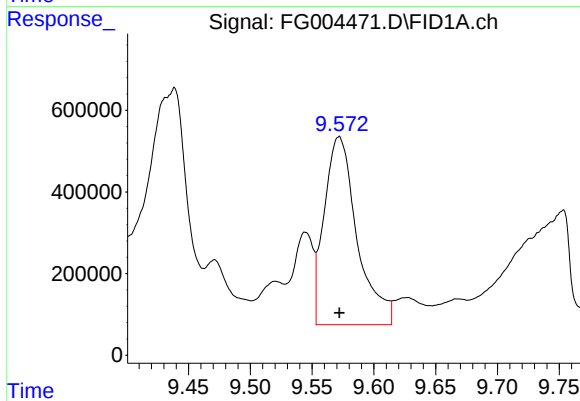

#5 N-HEXADECANE


R.T.: 9.572 min
Delta R.T.: 0.000 min
Response: 8501623
Conc: 75.99 ug/ml

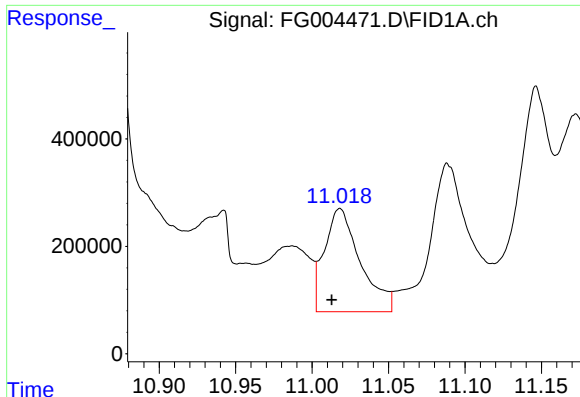

#6 N-OCTADECANE


R.T.: 11.018 min
Delta R.T.: 0.005 min
Response: 3134216
Conc: 27.63 ug/ml

Instrument :
FID_G
ClientSampleId :

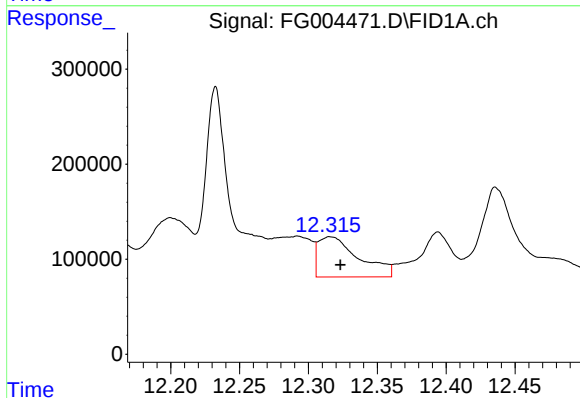


#7 N-EICOSANE

R.T.: 12.316 min
Delta R.T.: -0.007 min
Response: 862720
Conc: 7.55 ug/ml

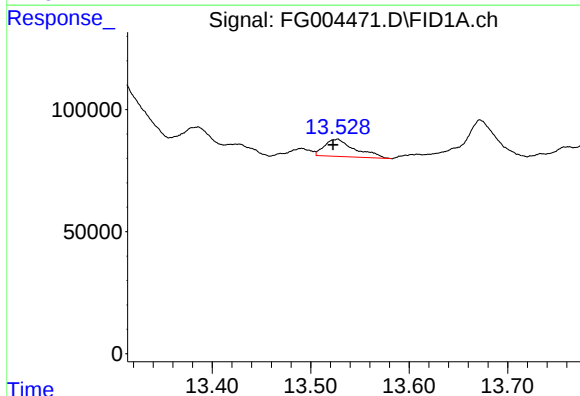


#8 N-DOCOSANE

R.T.: 13.527 min
Delta R.T.: 0.005 min
Response: 151786
Conc: 1.33 ug/ml

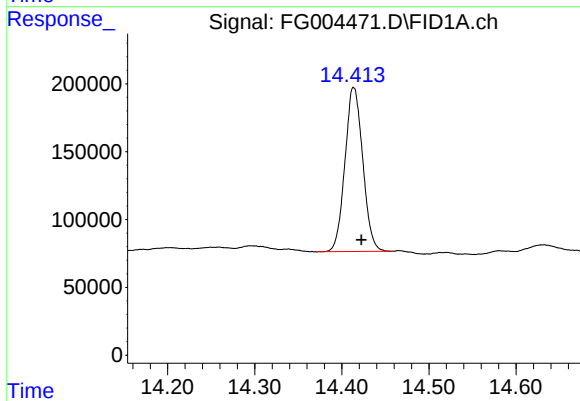

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.414 min
Delta R.T.: -0.009 min
Response: 1718198
Conc: 16.66 ug/ml

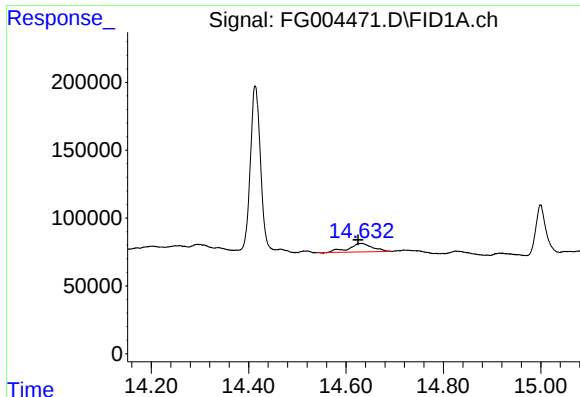

#10 N-TETRACOSANE


R.T.: 14.632 min
Delta R.T.: 0.007 min
Response: 214727
Conc: 1.86 ug/ml

Instrument :
FID_G
ClientSampleId :

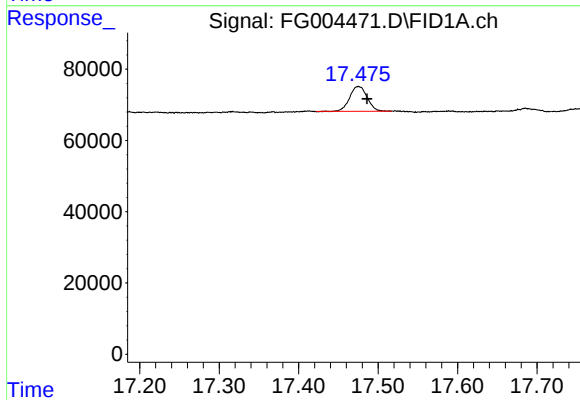

#13 N-TRIACONTANE

R.T.: 17.475 min
Delta R.T.: -0.011 min
Response: 106415
Conc: 0.90 ug/ml

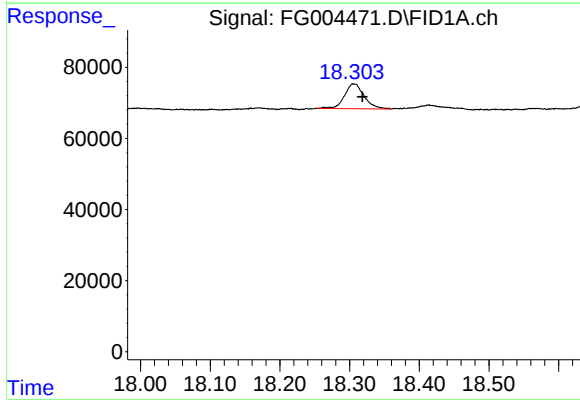

#14 N-DOTRIACONTANE

R.T.: 18.306 min
Delta R.T.: -0.013 min
Response: 135938
Conc: 1.16 ug/ml