

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
 Data File : FG004472.D
 Signal(s) : FID1A.ch
 Acq On : 30 Mar 2019 06:24
 Operator : AJ\SJ
 Sample : K2115-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 01 01:49:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.414	1938204	18.791 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.324	306389	2.613 ug/ml
16) N-HEXATRIACONTANE	19.877	807980	7.248 ug/ml
18) N-TETRACONTANE	21.404	1352683	12.505 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004472.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2019 06:24
Operator : AJ\SJ
Sample : K2115-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 01:49:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

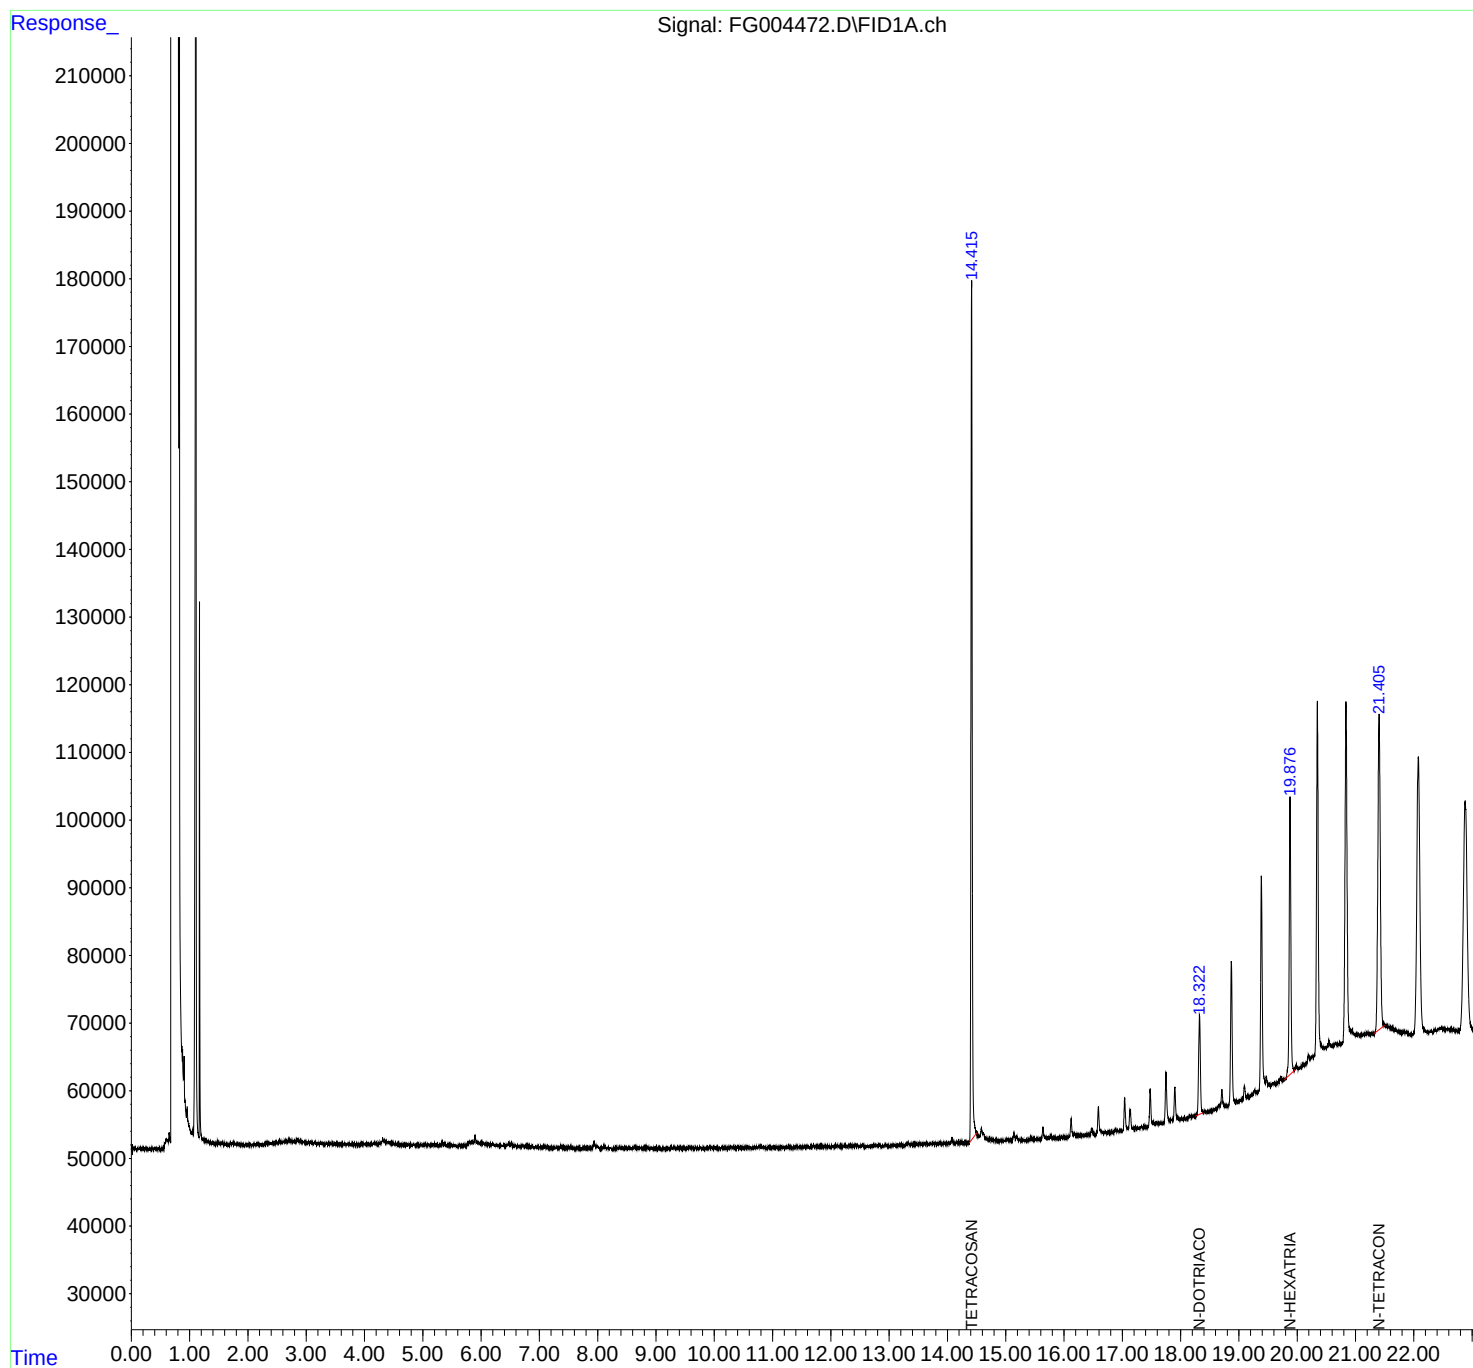


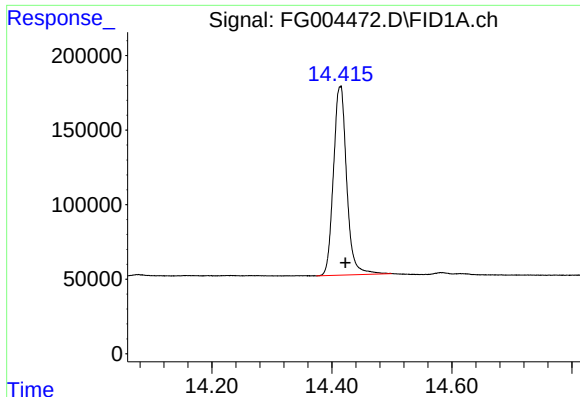

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.414 min
Delta R.T.: -0.008 min
Response: 1938204
Conc: 18.79 ug/ml

Instrument :
FID_G
ClientSampleId :

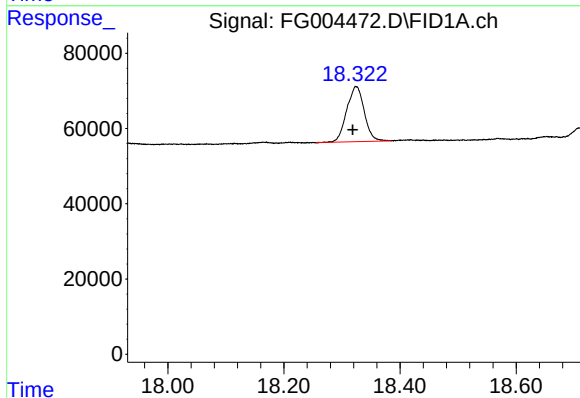


#14 N-DOTRIACONTANE

R.T.: 18.324 min
Delta R.T.: 0.006 min
Response: 306389
Conc: 2.61 ug/ml

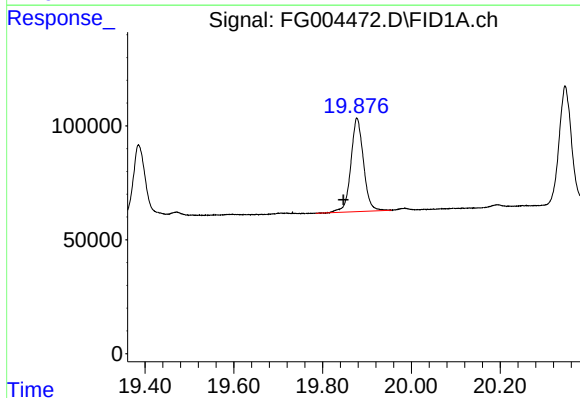

#16 N-HEXATRIACONTANE

R.T.: 19.877 min
Delta R.T.: 0.030 min
Response: 807980
Conc: 7.25 ug/ml

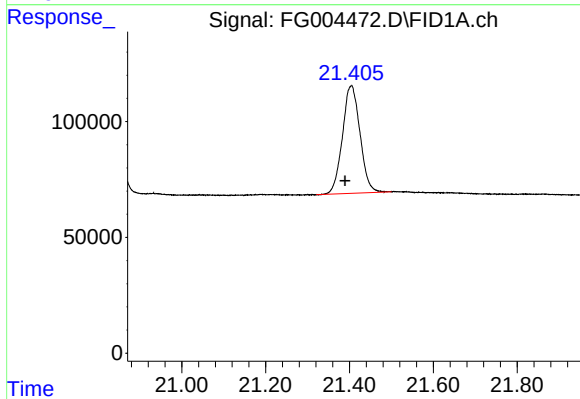

#18 N-TETRACONTANE

R.T.: 21.404 min
Delta R.T.: 0.015 min
Response: 1352683
Conc: 12.51 ug/ml