

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
 Data File : FG004476.D
 Signal(s) : FID1A.ch
 Acq On : 30 Mar 2019 08:25
 Operator : AJ\SJ
 Sample : K2115-03 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 01 01:50:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.412	150910	1.463 ug/ml
Target Compounds			
2) N-DECANE	4.189	692998	6.565 ug/ml
3) N-DODECANE	6.217	416488	3.953 ug/ml
4) N-TETRADECANE	7.958	249742	2.305 ug/ml
5) N-HEXADECANE	9.579	953513	8.523 ug/ml
6) N-OCTADECANE	11.022	270488	2.385 ug/ml
14) N-DOTRIACONTANE	18.322	139150	1.187 ug/ml
16) N-HEXATRIACONTANE	19.878	306133	2.746 ug/ml
18) N-TETRACONTANE	21.402	488633	4.517 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004476.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2019 08:25
Operator : AJ\SJ
Sample : K2115-03 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 01:50:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

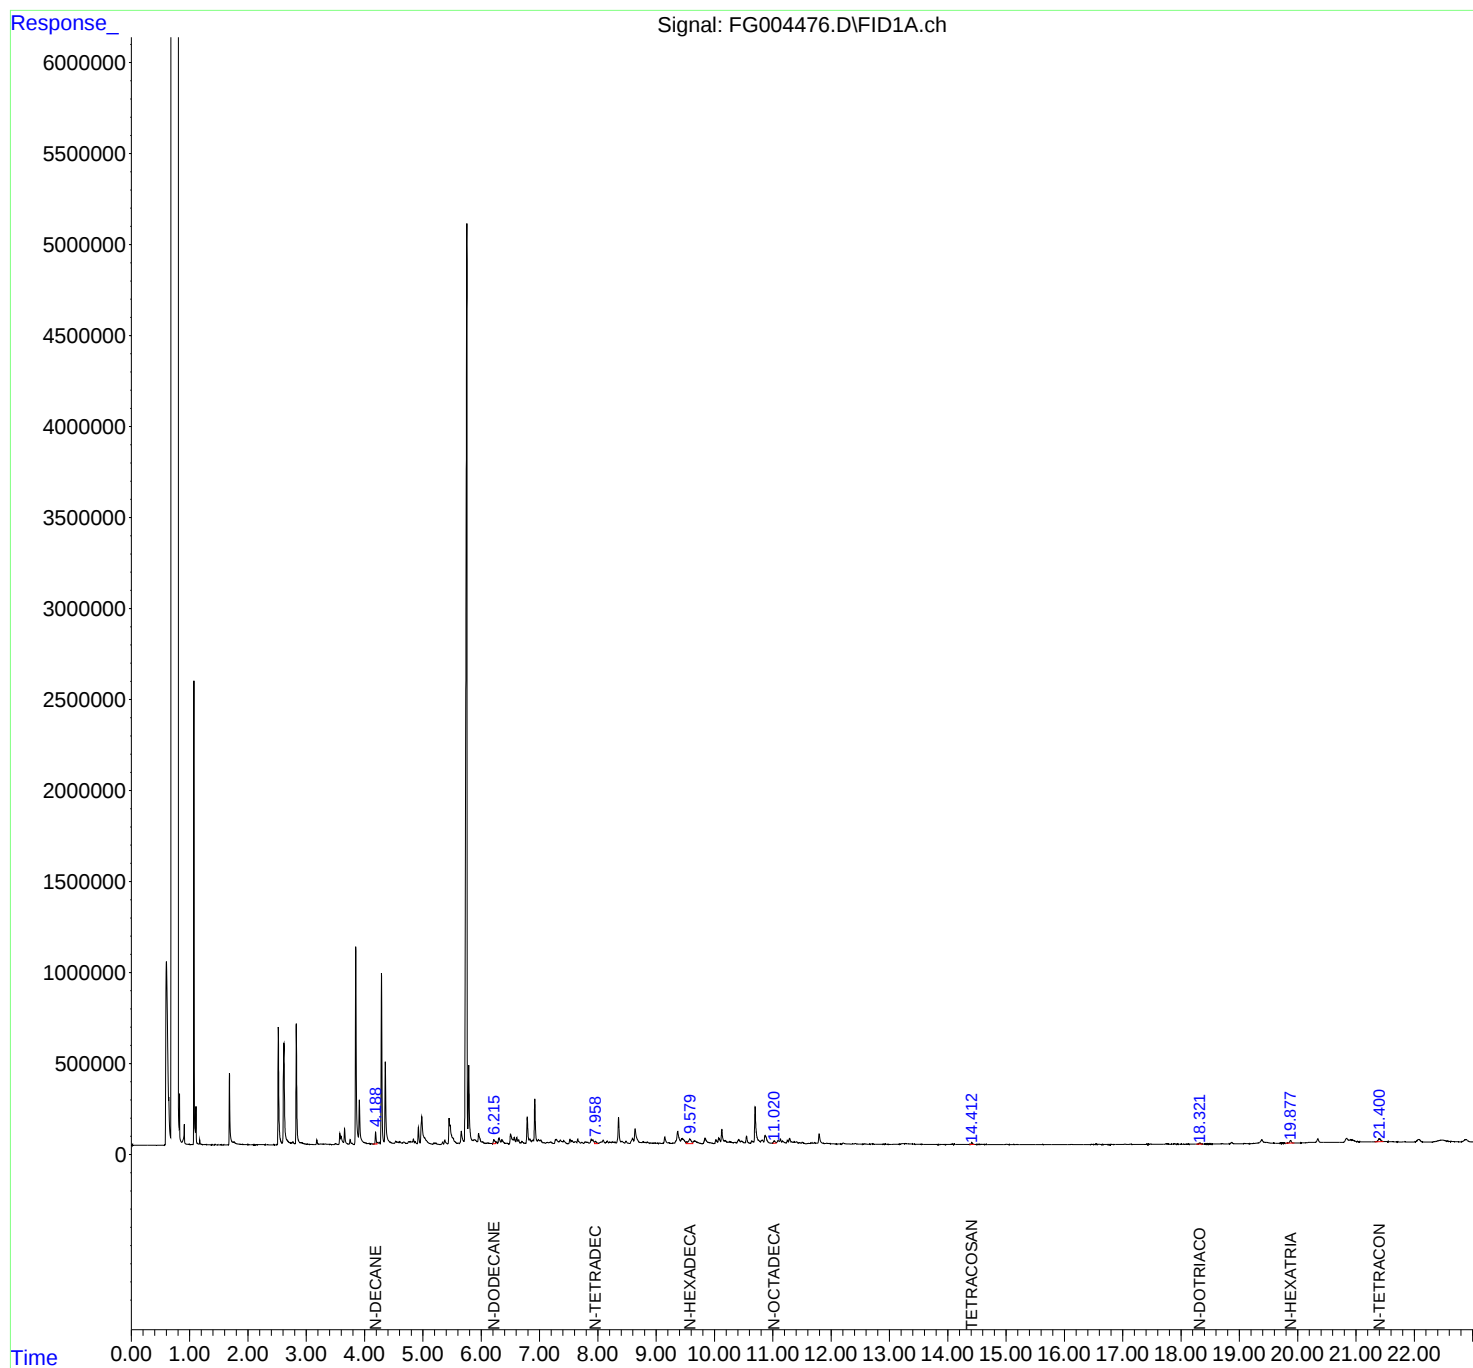


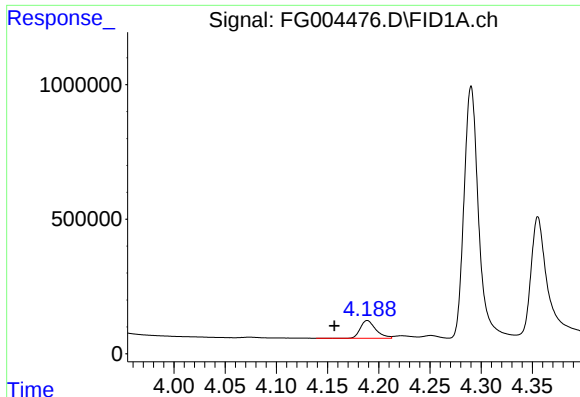

#2 N-DECANE


R.T.: 4.189 min
Delta R.T.: 0.032 min
Response: 692998
Conc: 6.57 ug/ml

Instrument :
FID_G
ClientSampleId :

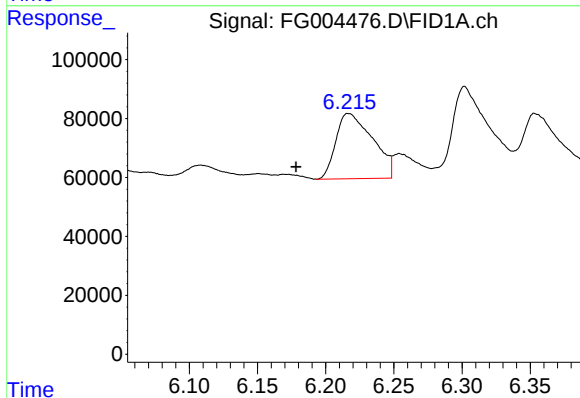


#3 N-DODECANE

R.T.: 6.217 min
Delta R.T.: 0.039 min
Response: 416488
Conc: 3.95 ug/ml

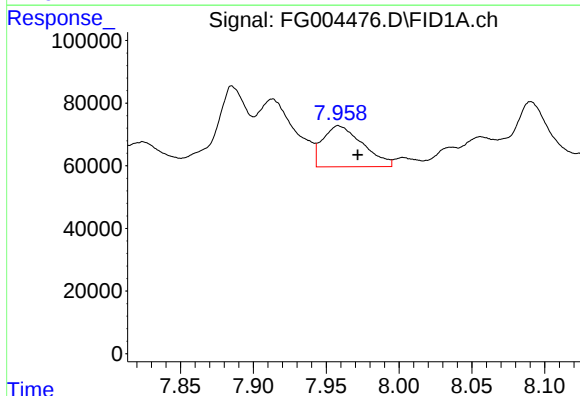


#4 N-TETRADECANE

R.T.: 7.958 min
Delta R.T.: -0.013 min
Response: 249742
Conc: 2.30 ug/ml

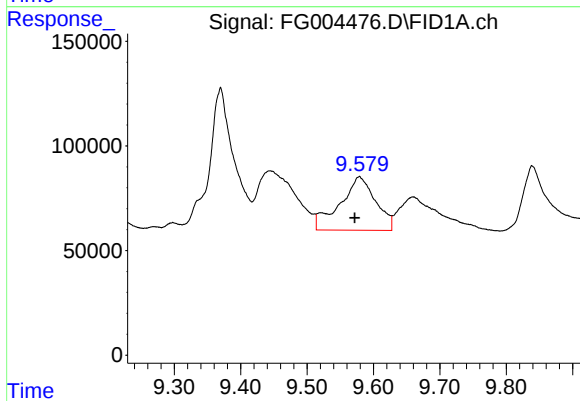

#5 N-HEXADECANE


R.T.: 9.579 min
Delta R.T.: 0.007 min
Response: 953513
Conc: 8.52 ug/ml

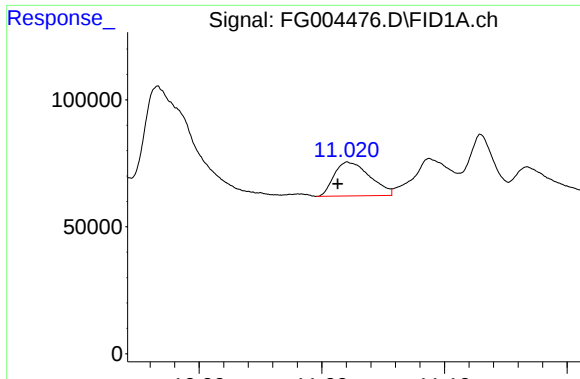

#6 N-OCTADECANE


R.T.: 11.022 min
Delta R.T.: 0.009 min
Response: 270488
Conc: 2.38 ug/ml

Instrument :
FID_G
ClientSampleId :

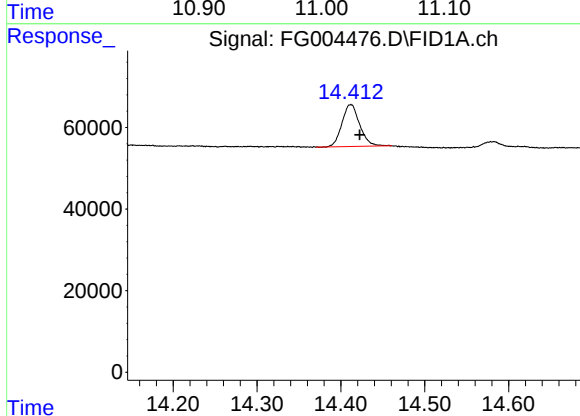


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.412 min
Delta R.T.: -0.011 min
Response: 150910
Conc: 1.46 ug/ml

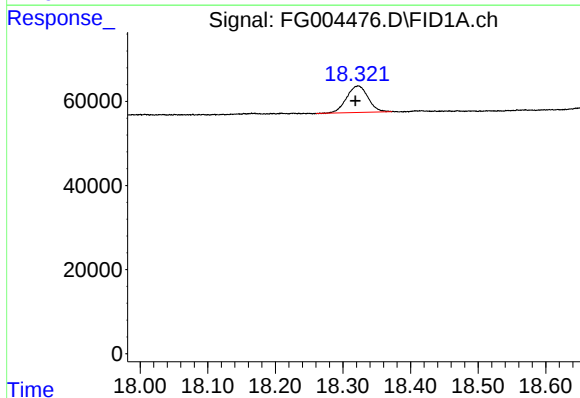


#14 N-DOTRIACONTANE

R.T.: 18.322 min
Delta R.T.: 0.004 min
Response: 139150
Conc: 1.19 ug/ml

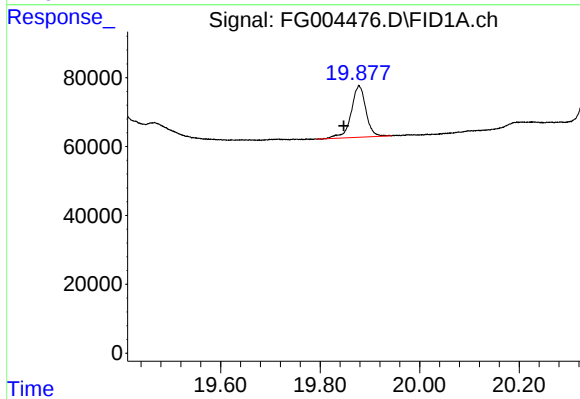

#16 N-HEXATRIACONTANE

R.T.: 19.878 min
Delta R.T.: 0.031 min
Response: 306133
Conc: 2.75 ug/ml

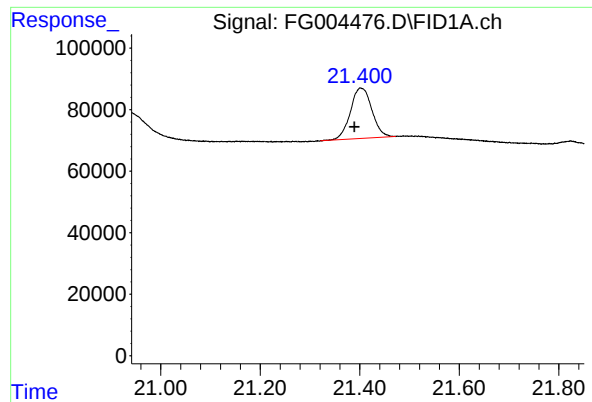

#18 N-TETRACONTANE

R.T.: 21.402 min
Delta R.T.: 0.013 min
Response: 488633
Conc: 4.52 ug/ml

Instrument :
FID_G
ClientSampleId :