

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004448.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2019 17:37
Operator : AJ\SJ
Sample : K2111-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S7A(4-20)COMP

Integration File: autoint1.e
Quant Time: Mar 30 01:22:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.415	1666702	16.158 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032919\
Data File : FG004448.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2019 17:37
Operator : AJ\SJ
Sample : K2111-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S7A(4-20)COMP

Integration File: autoint1.e
Quant Time: Mar 30 01:22:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

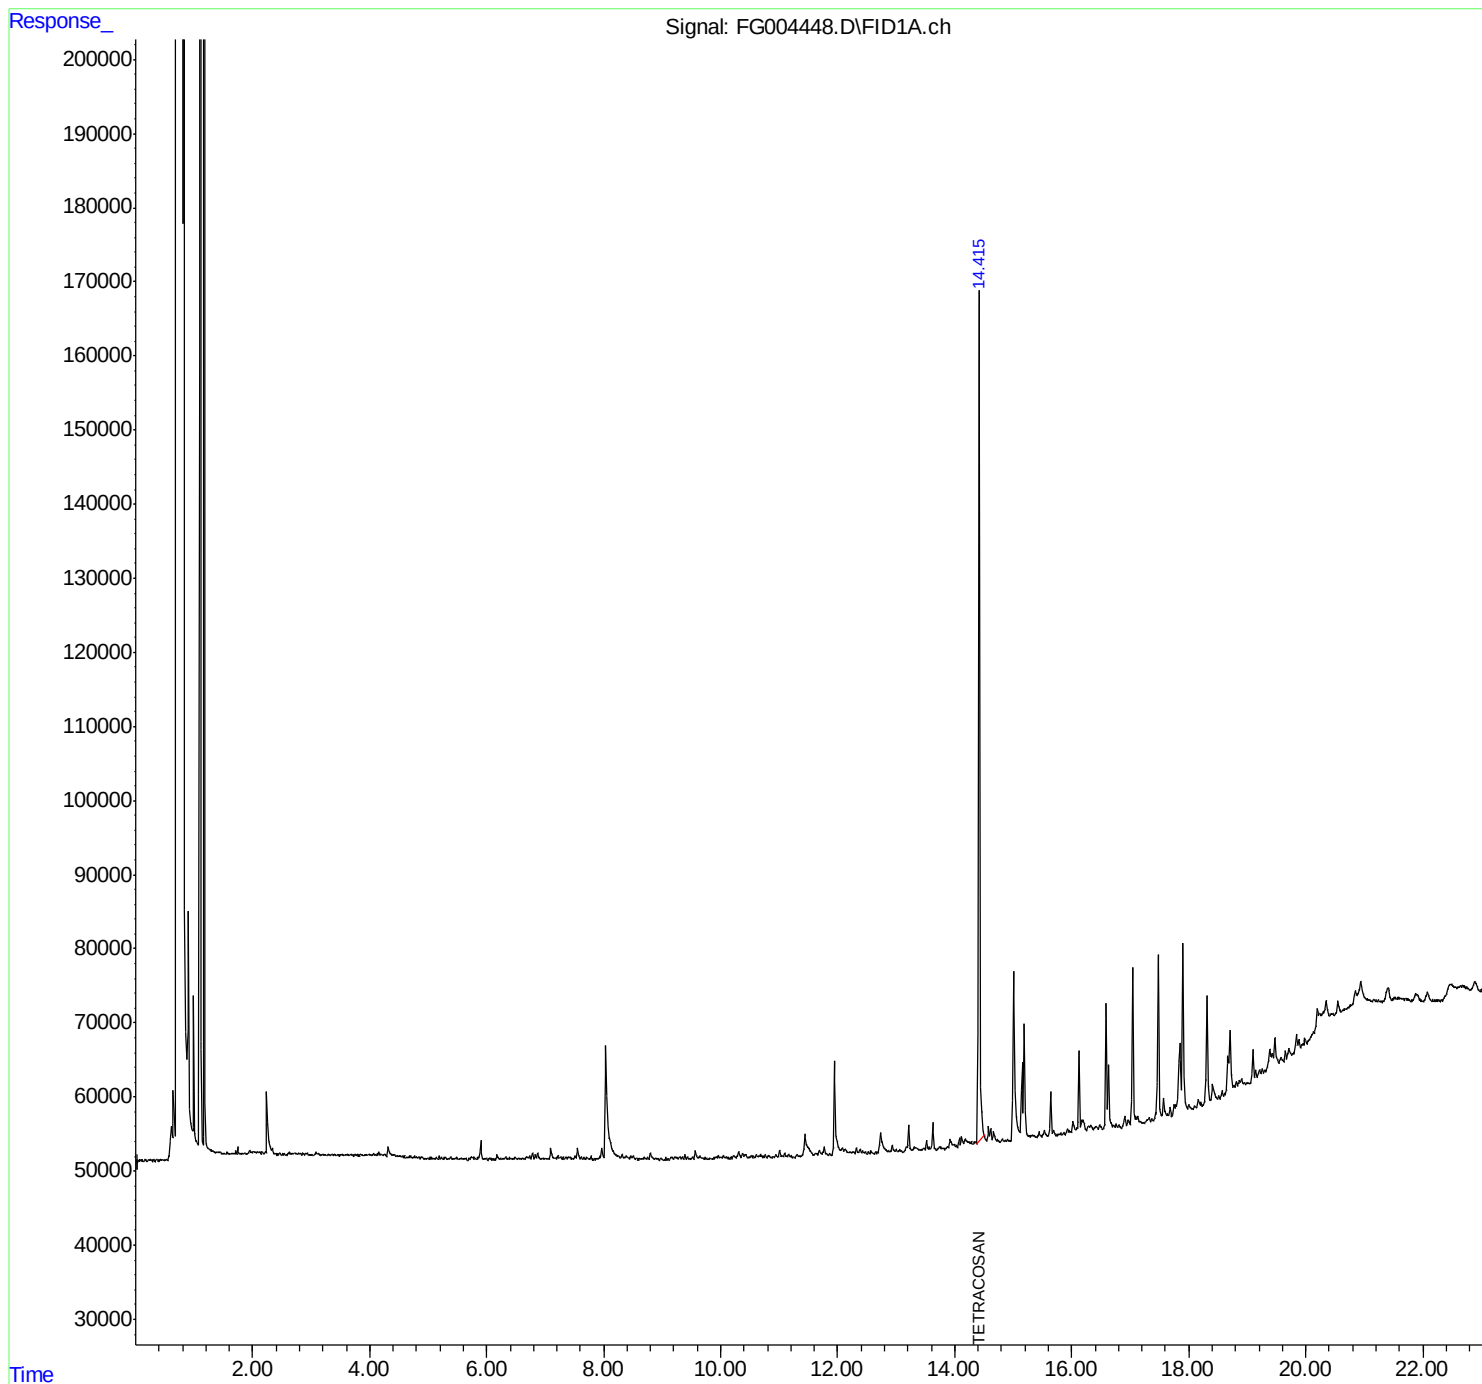

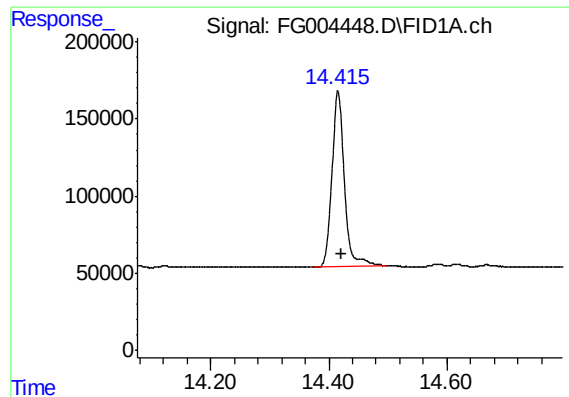

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.415 min
Delta R.T.: -0.007 min
Response: 1666702
Conc: 16.16 ug/ml

Instrument :
FID_G
ClientSampleId :
S7A(4-20)COMP