

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032923\
Data File : FG011686.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2023 13:41
Operator : YP\AJ
Sample : 02102-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CHAMBER-C-72-EAST

Integration File: autoint1.e
Quant Time: Mar 29 18:01:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.046	1866612	18.545 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032923\
Data File : FG011686.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2023 13:41
Operator : YP\AJ
Sample : 02102-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CHAMBER-C-72-EAST

Integration File: autoint1.e
Quant Time: Mar 29 18:01:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

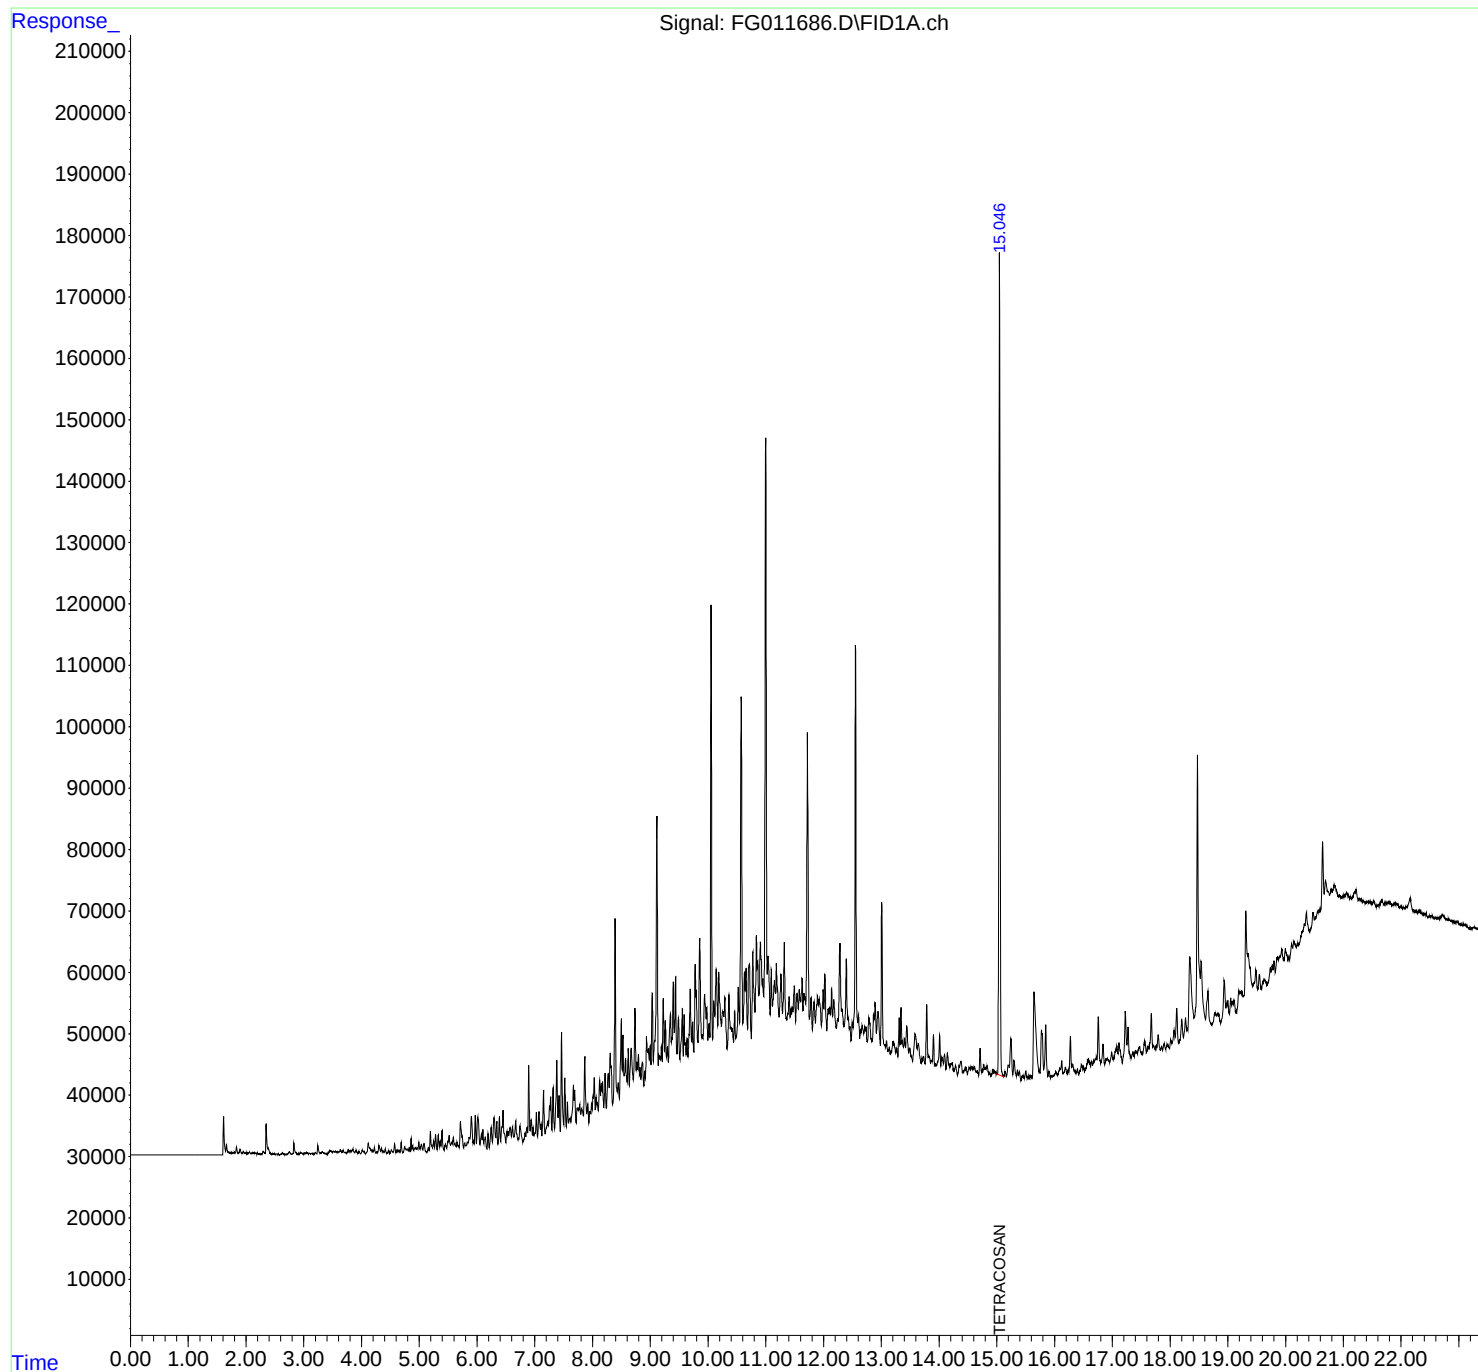

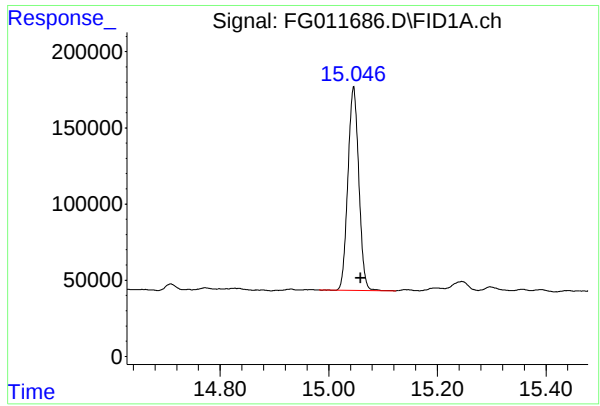

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.046 min
Delta R.T.: -0.013 min
Response: 1866612
Conc: 18.54 ug/ml

Instrument :
FID_G
ClientSampleId :
CHAMBER-C-72-EAST