

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032924\
Data File : FG013657.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2024 08:22
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 30 00:58:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031524.M
Quant Title :
QLast Update : Fri Mar 15 13:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.068	1931738	16.606 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032924\
Data File : FG013657.D
Signal(s) : FID1A.ch
Acq On : 29 Mar 2024 08:22
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 30 00:58:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031524.M
Quant Title :
QLast Update : Fri Mar 15 13:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

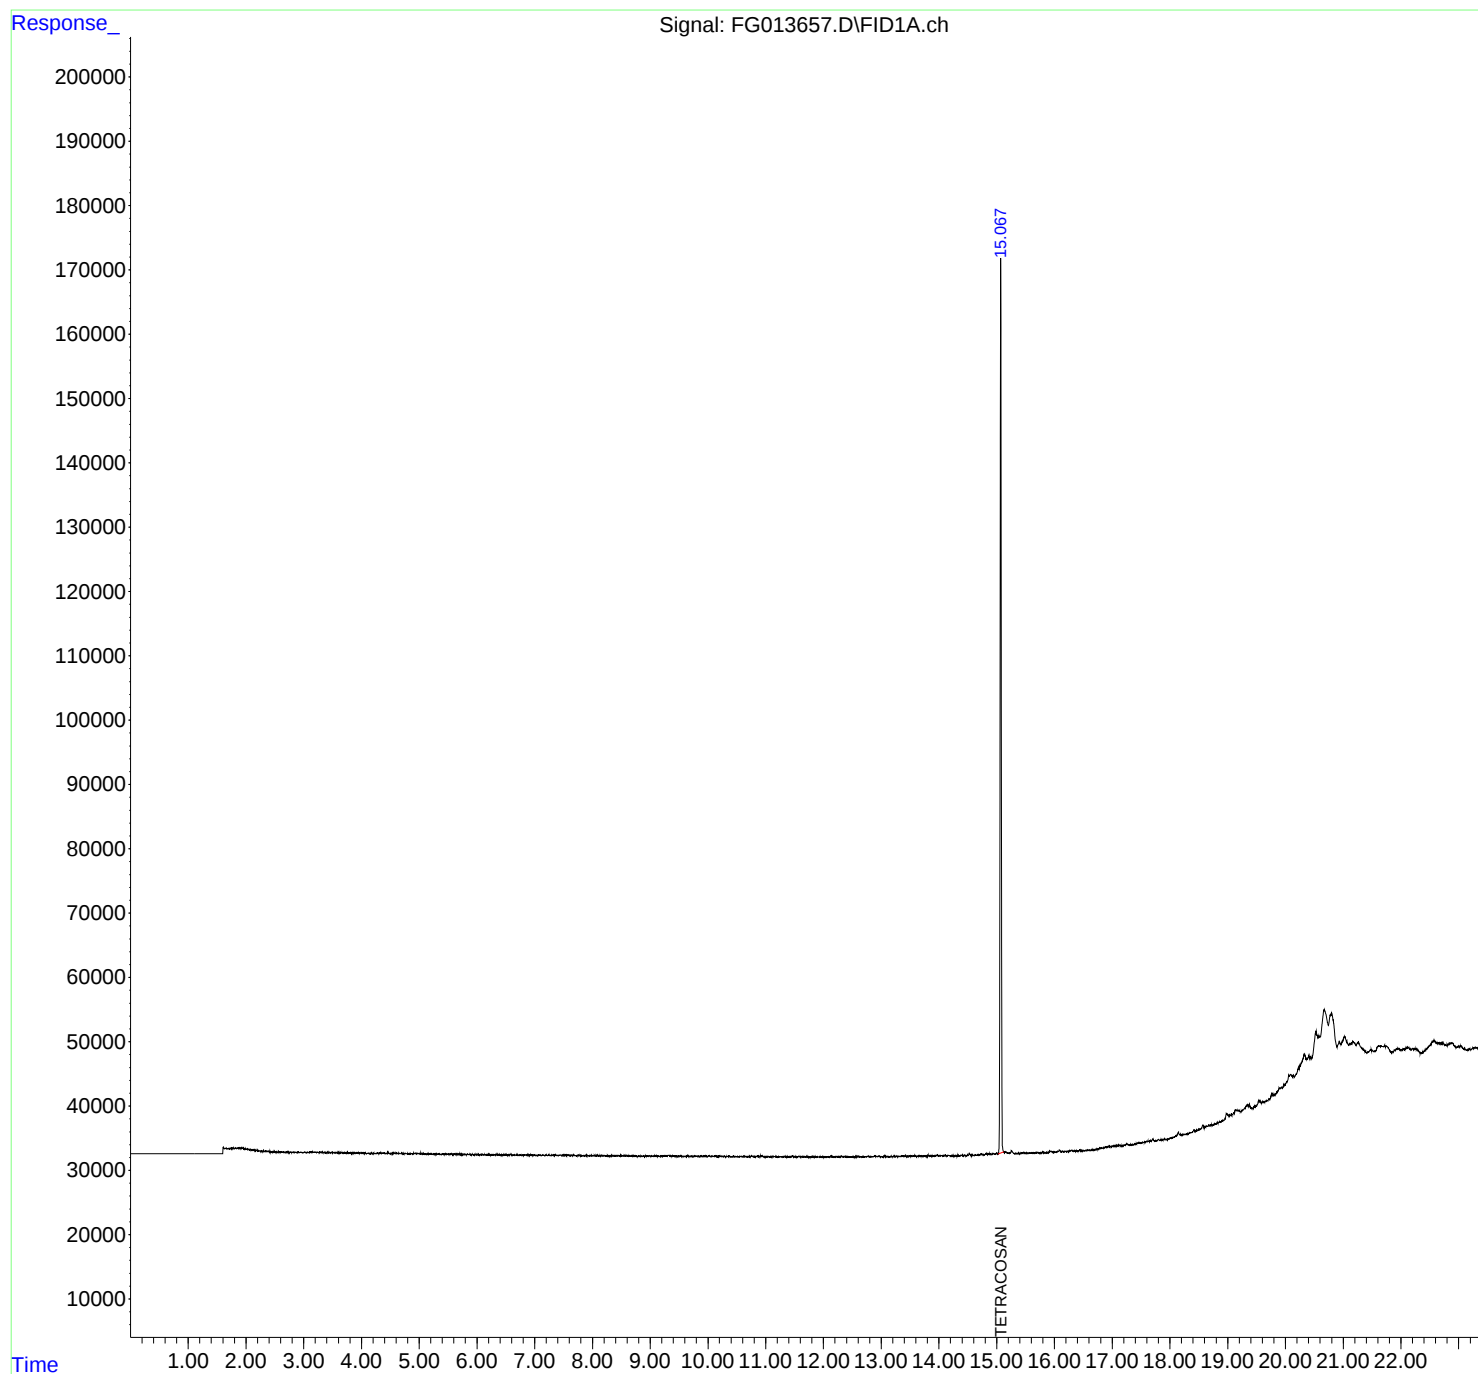

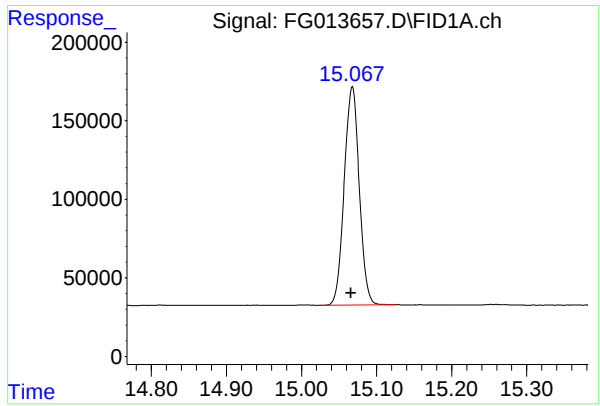

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.068 min
Delta R.T.: 0.002 min
Response: 1931738
Conc: 16.61 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK