

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG033023\
Data File : FG011706.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2023 18:42
Operator : YP\AJ
Sample : 02126-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RS-D

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2023
Supervised By :mohammad ahmed 03/31/2023

Integration File: Sample.e
Quant Time: Mar 31 00:40:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.073	2922431	29.035 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG033023\
Data File : FG011706.D
Signal(s) : FID1A.ch
Acq On : 30 Mar 2023 18:42
Operator : YP\AJ
Sample : 02126-04
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
RS-D


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2023
Supervised By :mohammad ahmed 03/31/2023

Integration File: Sample.e
Quant Time: Mar 31 00:40:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

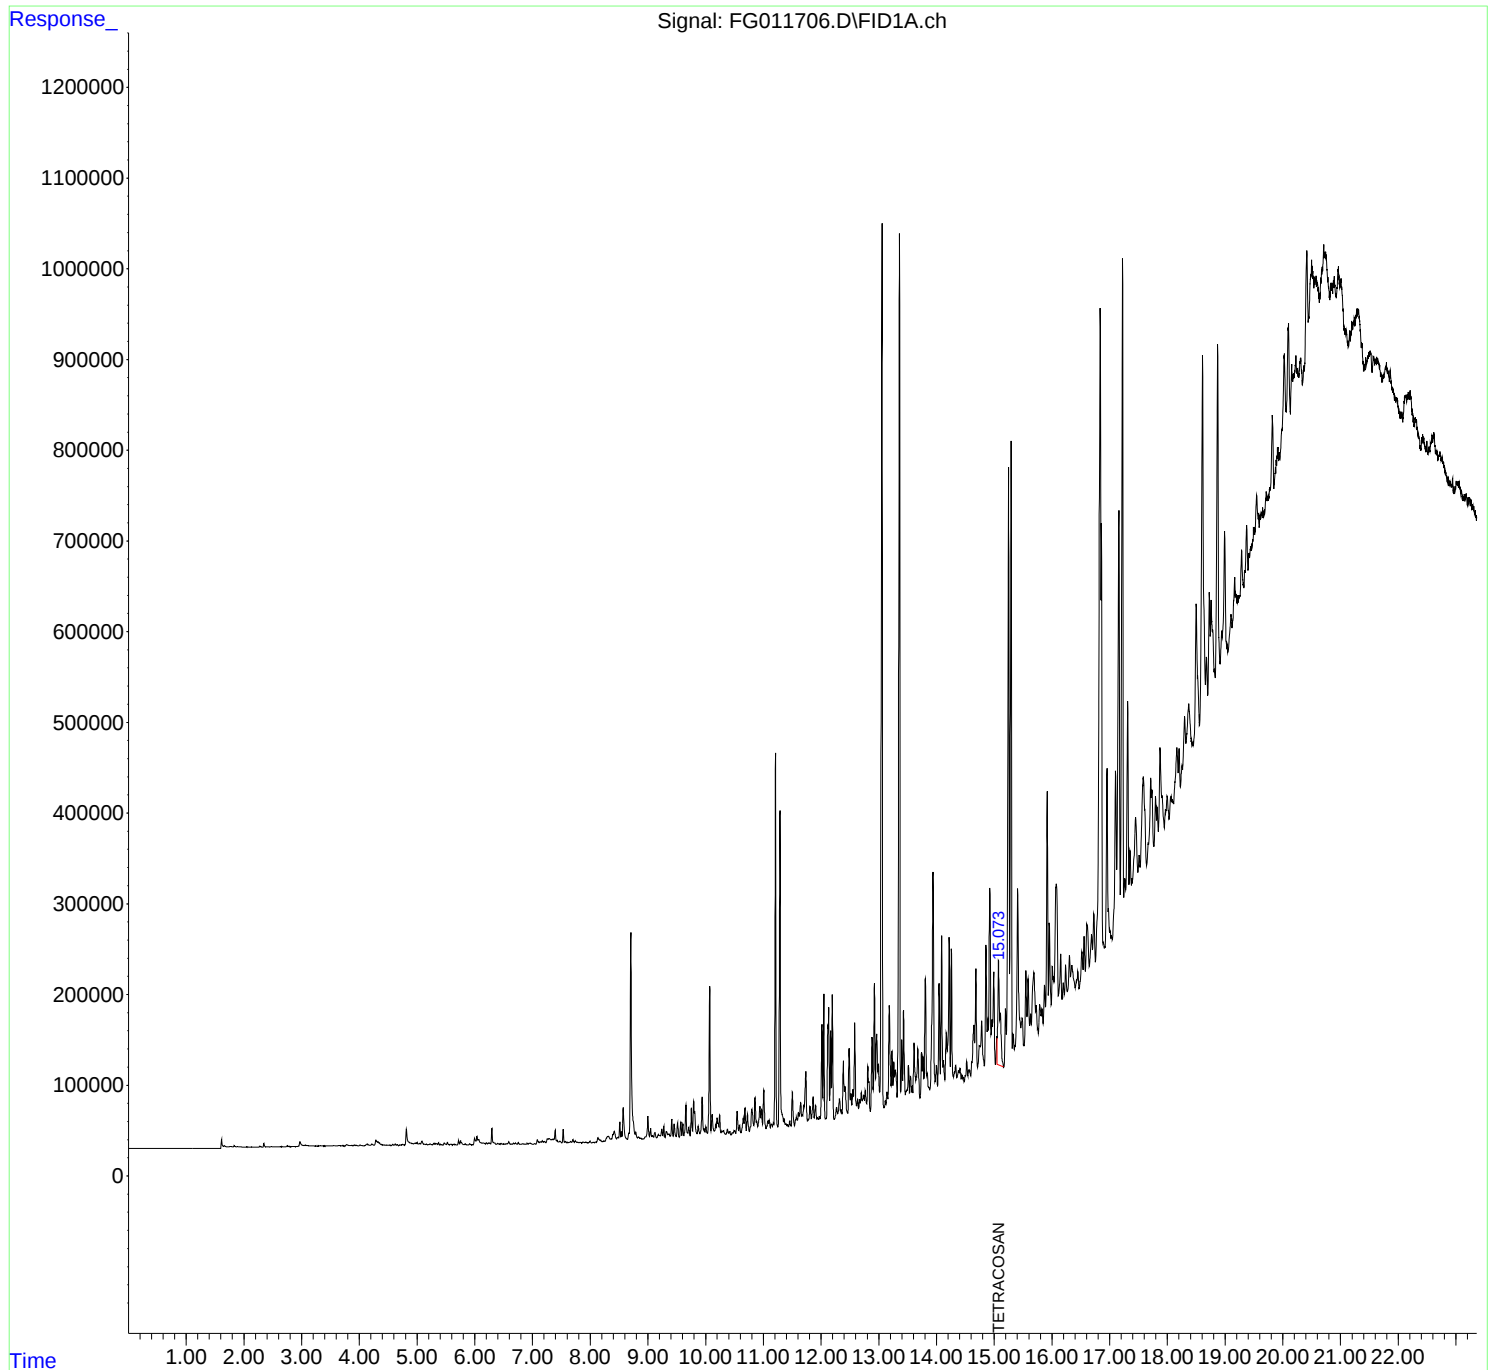

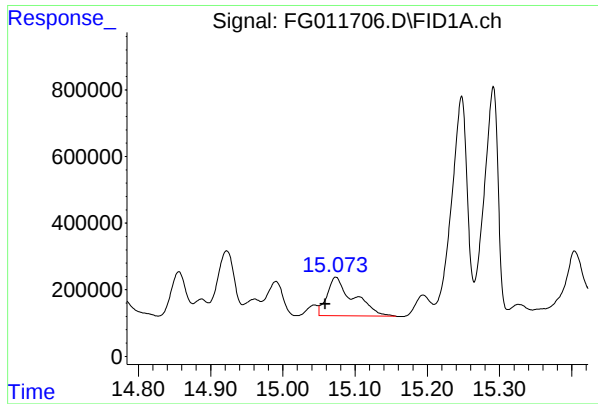

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.073 min
Delta R.T.: 0.013 min
Response: 2922431
Conc: 29.03 ug/ml

Instrument :
FID_G
ClientSampleId :
RS-D

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2023
Supervised By :mohammad ahmed 03/31/2023