

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
 Data File : FG004488.D
 Signal(s) : FID1A.ch
 Acq On : 01 Apr 2019 15:00
 Operator : AJ\SJ
 Sample : K1685-09 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 AU-06-032819-A

Integration File: autoint1.e
 Quant Time: Apr 02 00:43:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.410	340449	3.301 ug/ml
Target Compounds			
8) N-DOCOSANE	13.567	177220	1.550 ug/ml
10) N-TETRACOSANE	14.621	343081	2.970 ug/ml
12) N-OCTACOSANE	16.584	82624	0.714 ug/ml
14) N-DOTRIACONTANE	18.306	184476	1.573 ug/ml
15) N-TETRATRIACONTANE	19.090	153144	1.374 ug/ml
16) N-HEXATRIACONTANE	19.836	96124	0.862 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004488.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 15:00
Operator : AJ\SJ
Sample : K1685-09 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-032819-A

Integration File: autoint1.e
Quant Time: Apr 02 00:43:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

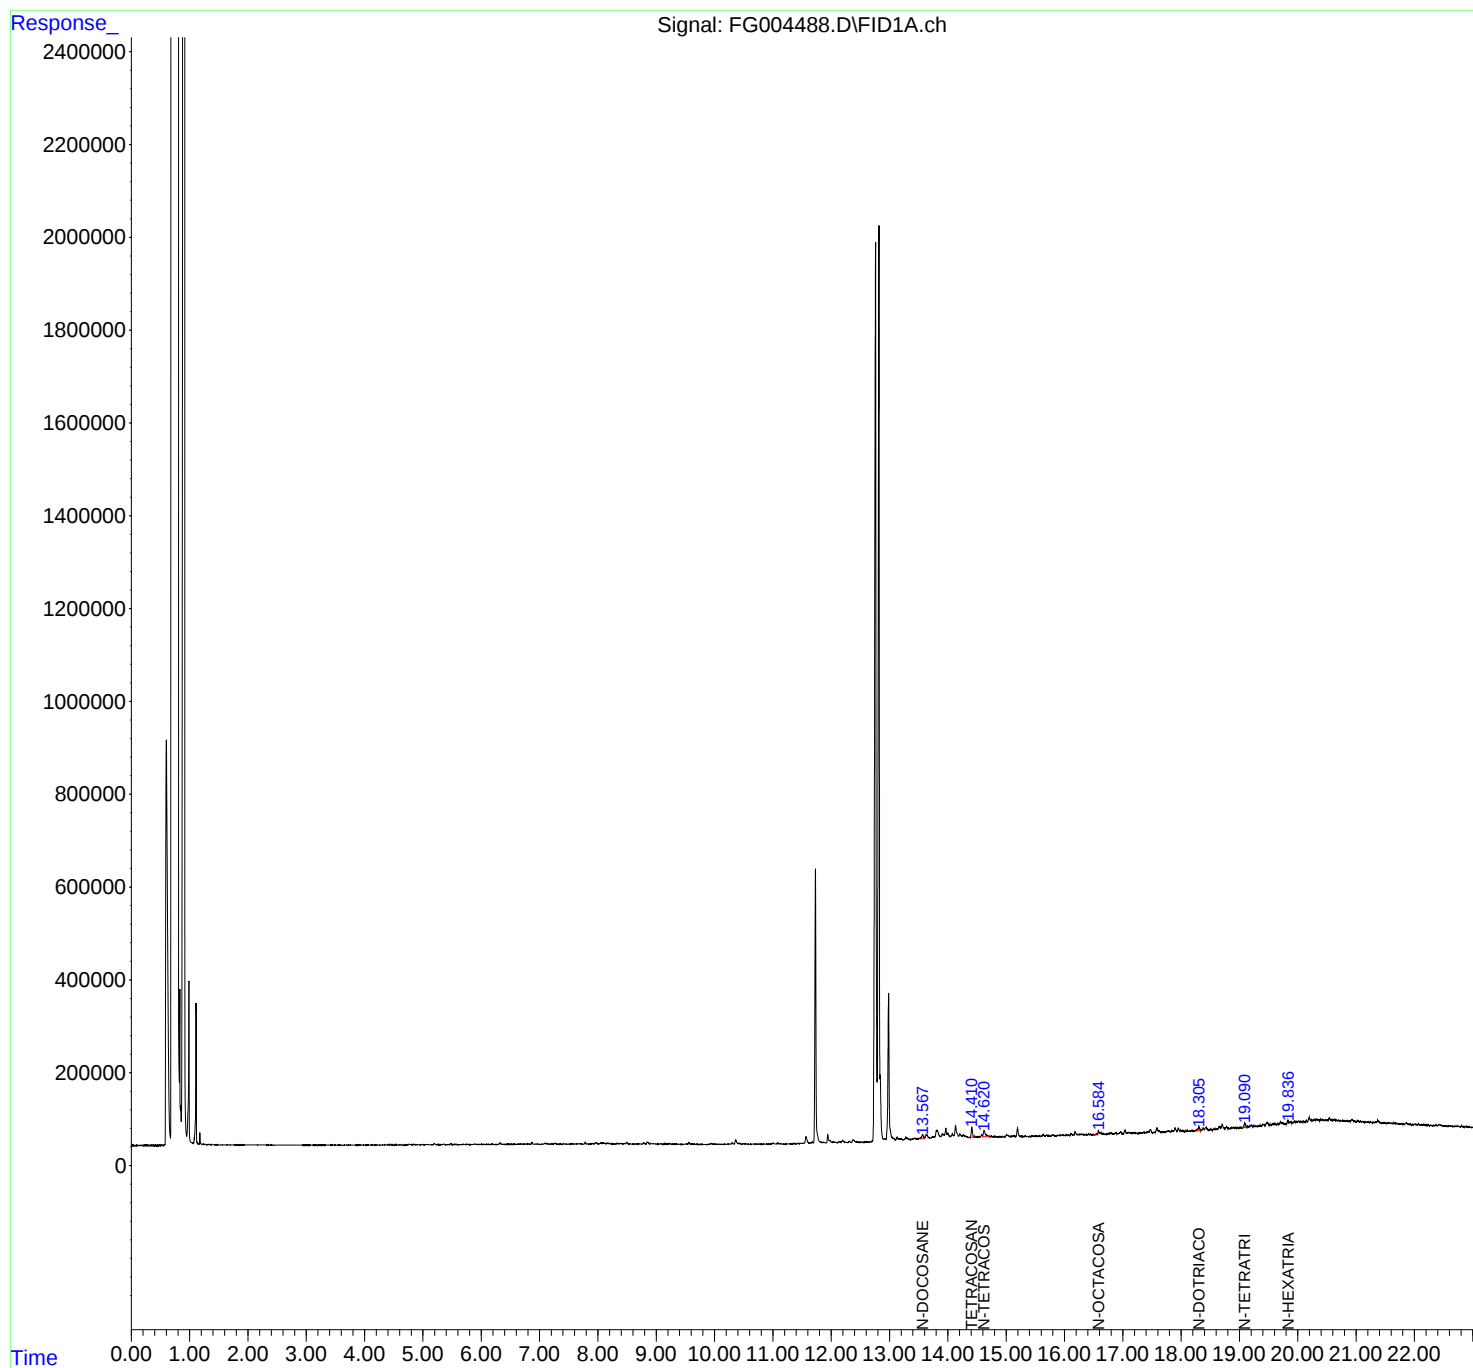


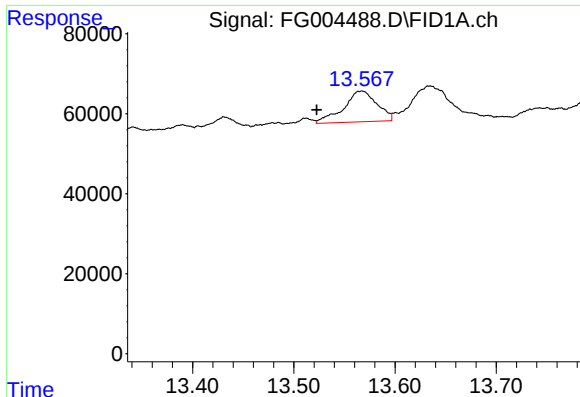

#8 N-DOCOSANE


R.T.: 13.567 min
Delta R.T.: 0.045 min
Response: 177220
Conc: 1.55 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-A

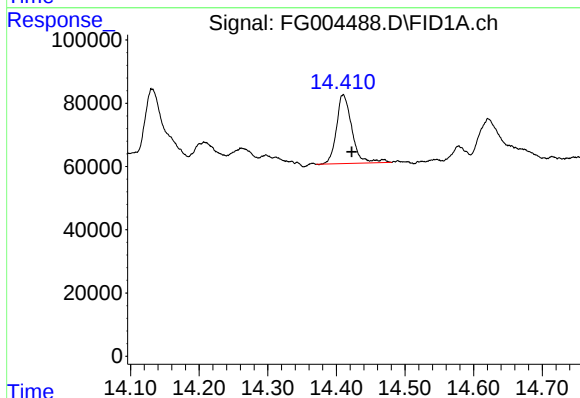


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.410 min
Delta R.T.: -0.013 min
Response: 340449
Conc: 3.30 ug/ml

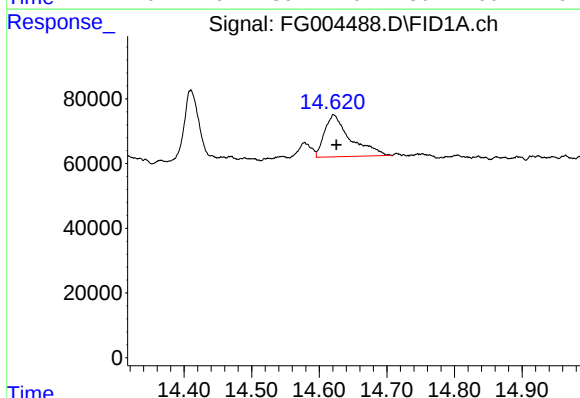


#10 N-TETRACOSANE

R.T.: 14.621 min
Delta R.T.: -0.004 min
Response: 343081
Conc: 2.97 ug/ml

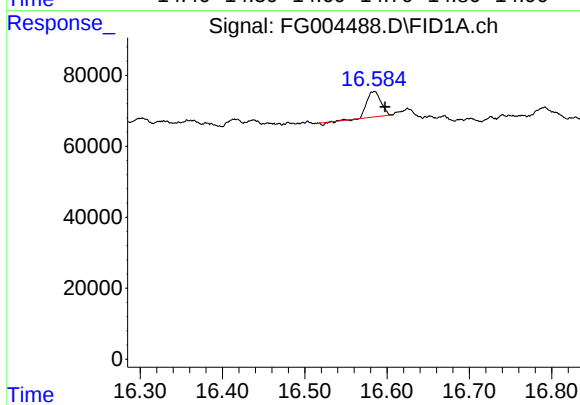

#12 N-OCTACOSANE


R.T.: 16.584 min
Delta R.T.: -0.013 min
Response: 82624
Conc: 0.71 ug/ml

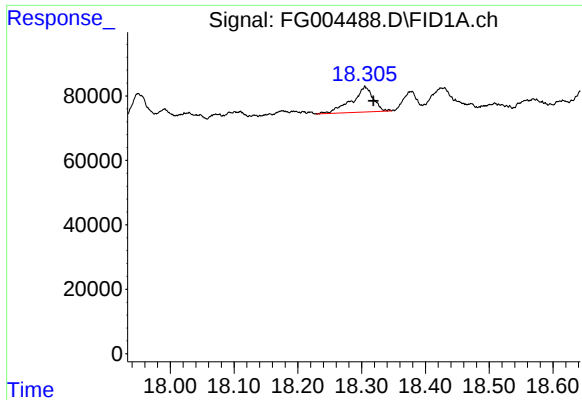

#14 N-DOTRIACONTANE


R.T.: 18.306 min
Delta R.T.: -0.013 min
Response: 184476
Conc: 1.57 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-A

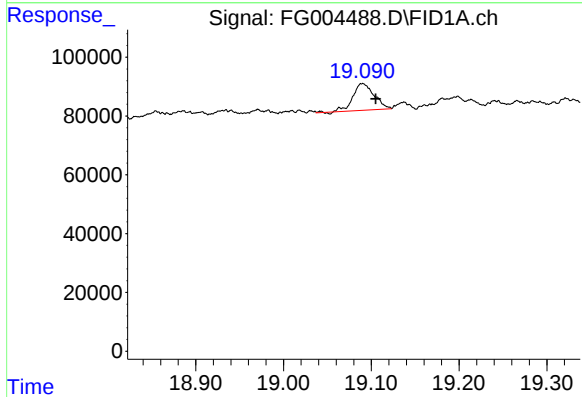

#15 N-TETRATRIACONTANE

R.T.: 19.090 min
Delta R.T.: -0.015 min
Response: 153144
Conc: 1.37 ug/ml

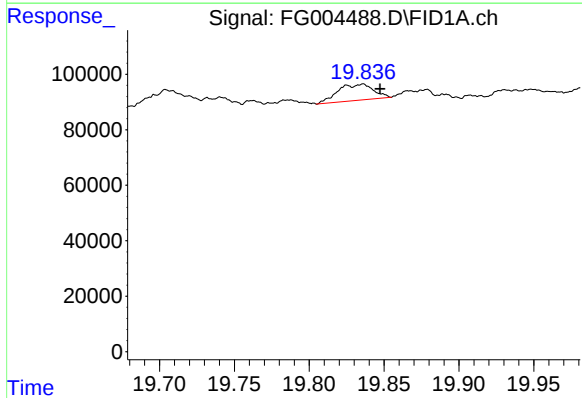

#16 N-HEXATRIACONTANE

R.T.: 19.836 min
Delta R.T.: -0.011 min
Response: 96124
Conc: 0.86 ug/ml