

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
 Data File : FG004489.D
 Signal(s) : FID1A.ch
 Acq On : 01 Apr 2019 15:30
 Operator : AJ\SJ
 Sample : K1685-11 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 AU-06-032819-B

Integration File: autoint1.e
 Quant Time: Apr 02 00:44:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.410	191246	1.854 ug/ml
Target Compounds			
7) N-EICOSANE	12.392f	407688	3.566 ug/ml
8) N-DOCOSANE	13.563	338251	2.959 ug/ml
10) N-TETRACOSANE	14.616	765076	6.623 ug/ml
12) N-OCTACOSANE	16.584	131307	1.135 ug/ml
13) N-TRIACONTANE	17.473	149604	1.261 ug/ml
14) N-DOTRIACONTANE	18.308	220335	1.879 ug/ml
15) N-TETRATRIACONTANE	19.092	123803	1.111 ug/ml
16) N-HEXATRIACONTANE	19.835	108728	0.975 ug/ml
18) N-TETRACONTANE	21.407	383760	3.548 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004489.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 15:30
Operator : AJ\SJ
Sample : K1685-11 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

Integration File: autoint1.e
Quant Time: Apr 02 00:44:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

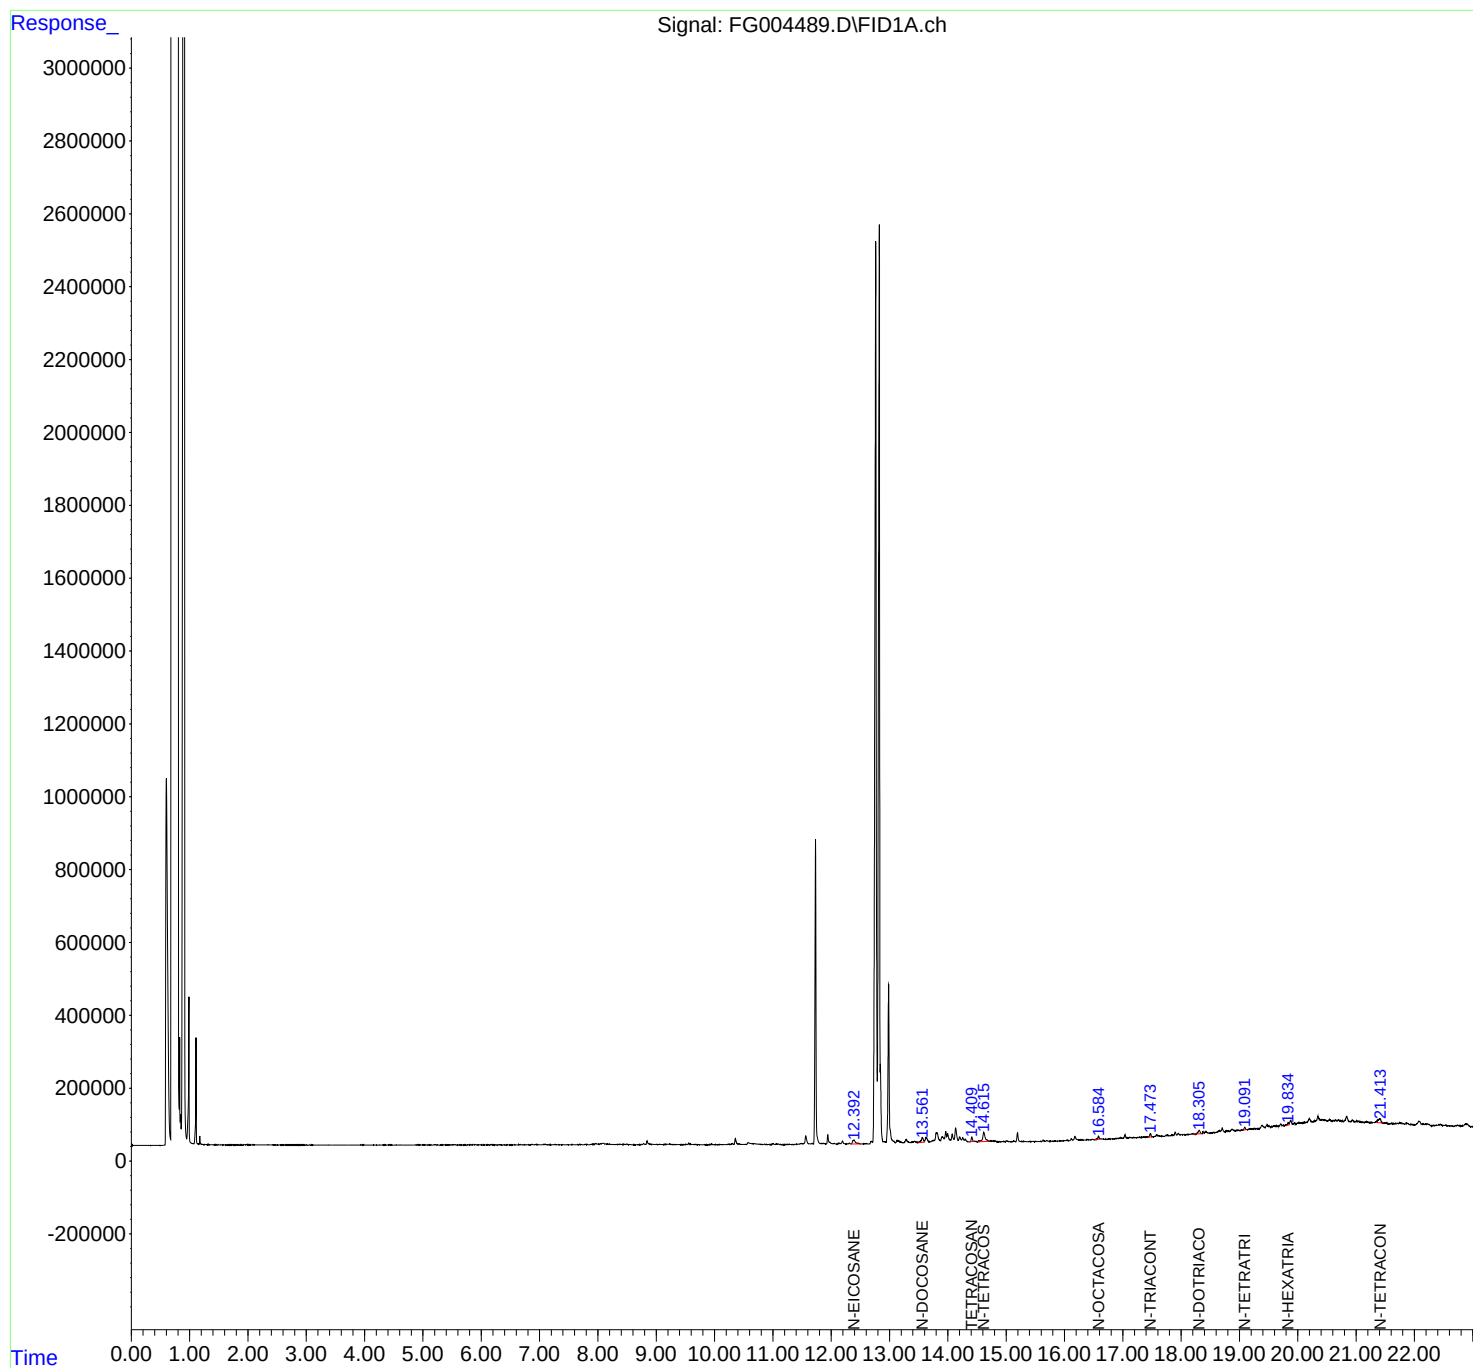


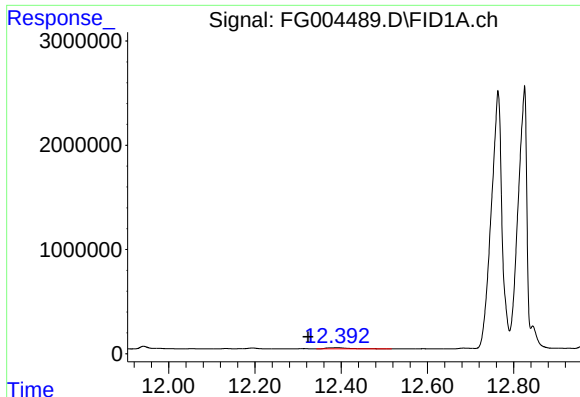

#7 N-EICOSANE


R.T.: 12.392 min
Delta R.T.: 0.069 min
Response: 407688
Conc: 3.57 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

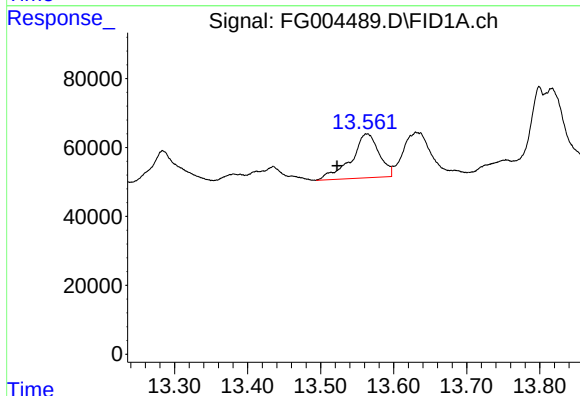


#8 N-DOCOSANE

R.T.: 13.563 min
Delta R.T.: 0.041 min
Response: 338251
Conc: 2.96 ug/ml

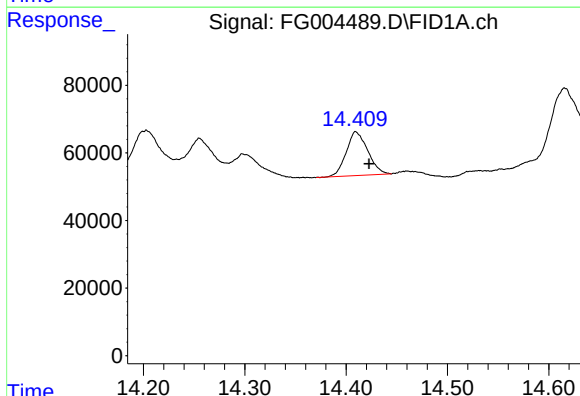


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.410 min
Delta R.T.: -0.013 min
Response: 191246
Conc: 1.85 ug/ml

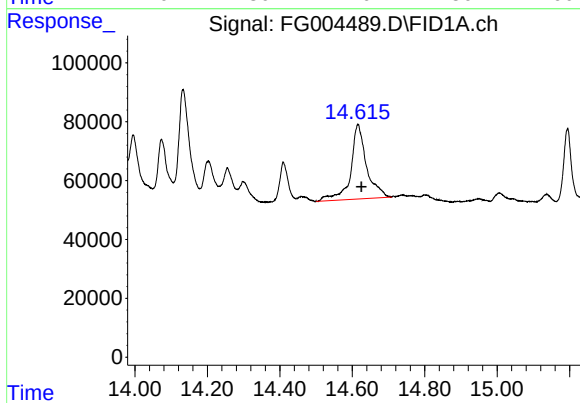

#10 N-TETRACOSANE


R.T.: 14.616 min
Delta R.T.: -0.009 min
Response: 765076
Conc: 6.62 ug/ml

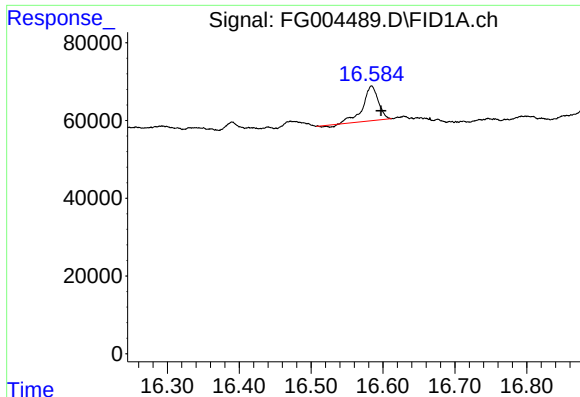

#12 N-OCTACOSANE


R.T.: 16.584 min
Delta R.T.: -0.013 min
Response: 131307
Conc: 1.14 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

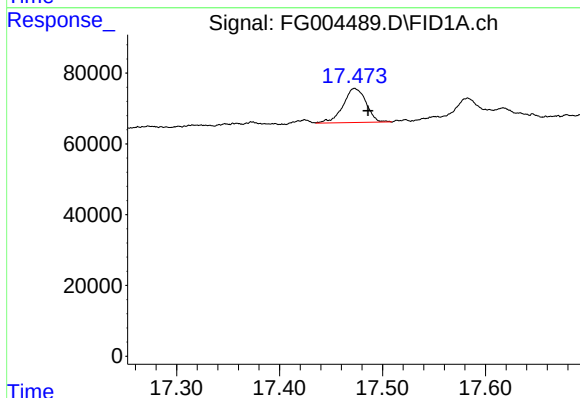


#13 N-TRIACONTANE

R.T.: 17.473 min
Delta R.T.: -0.013 min
Response: 149604
Conc: 1.26 ug/ml

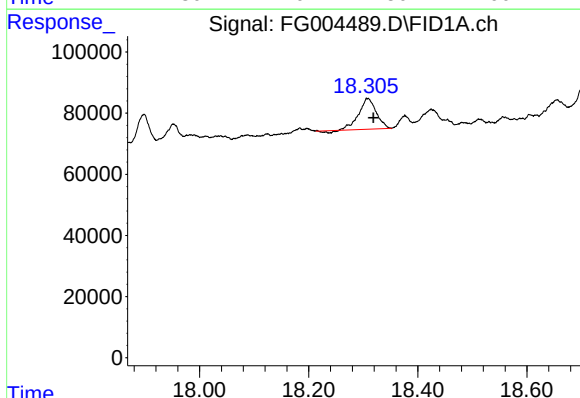


#14 N-DOTRIACONTANE

R.T.: 18.308 min
Delta R.T.: -0.010 min
Response: 220335
Conc: 1.88 ug/ml

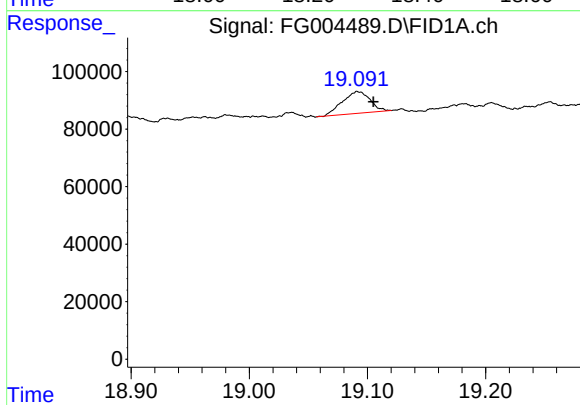

#15 N-TETRATRIACONTANE


R.T.: 19.092 min
Delta R.T.: -0.013 min
Response: 123803
Conc: 1.11 ug/ml

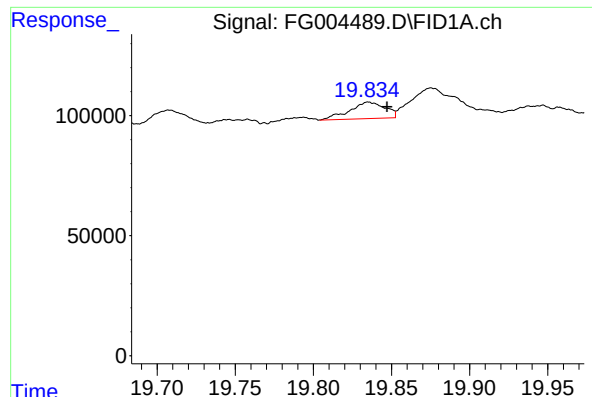

#16 N-HEXATRIACONTANE

R.T.: 19.835 min
Delta R.T.: -0.012 min
Response: 108728
Conc: 0.98 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

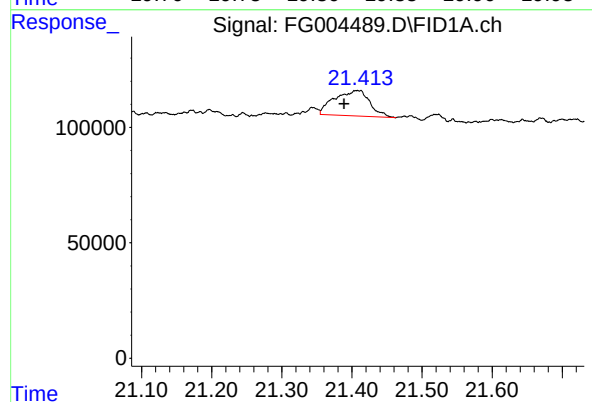

#18 N-TETRACONTANE

R.T.: 21.407 min
Delta R.T.: 0.018 min
Response: 383760
Conc: 3.55 ug/ml