

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
 Data File : FG004490.D
 Signal(s) : FID1A.ch
 Acq On : 01 Apr 2019 16:01
 Operator : AJ\SJ
 Sample : K1685-13 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 AU-06-032819-C

Integration File: autoint1.e
 Quant Time: Apr 02 00:44:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.410	132226	1.282 ug/ml
Target Compounds				
12)	N-OCTACOSANE	16.586	186155	1.609 ug/ml
13)	N-TRIACONTANE	17.476	165541	1.395 ug/ml
14)	N-DOTRIACONTANE	18.310	148244	1.264 ug/ml
15)	N-TETRATRIACONTANE	19.091	320961	2.881 ug/ml
16)	N-HEXATRIACONTANE	19.836	93512	0.839 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004490.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 16:01
Operator : AJ\SJ
Sample : K1685-13 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-032819-C

Integration File: autoint1.e
Quant Time: Apr 02 00:44:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

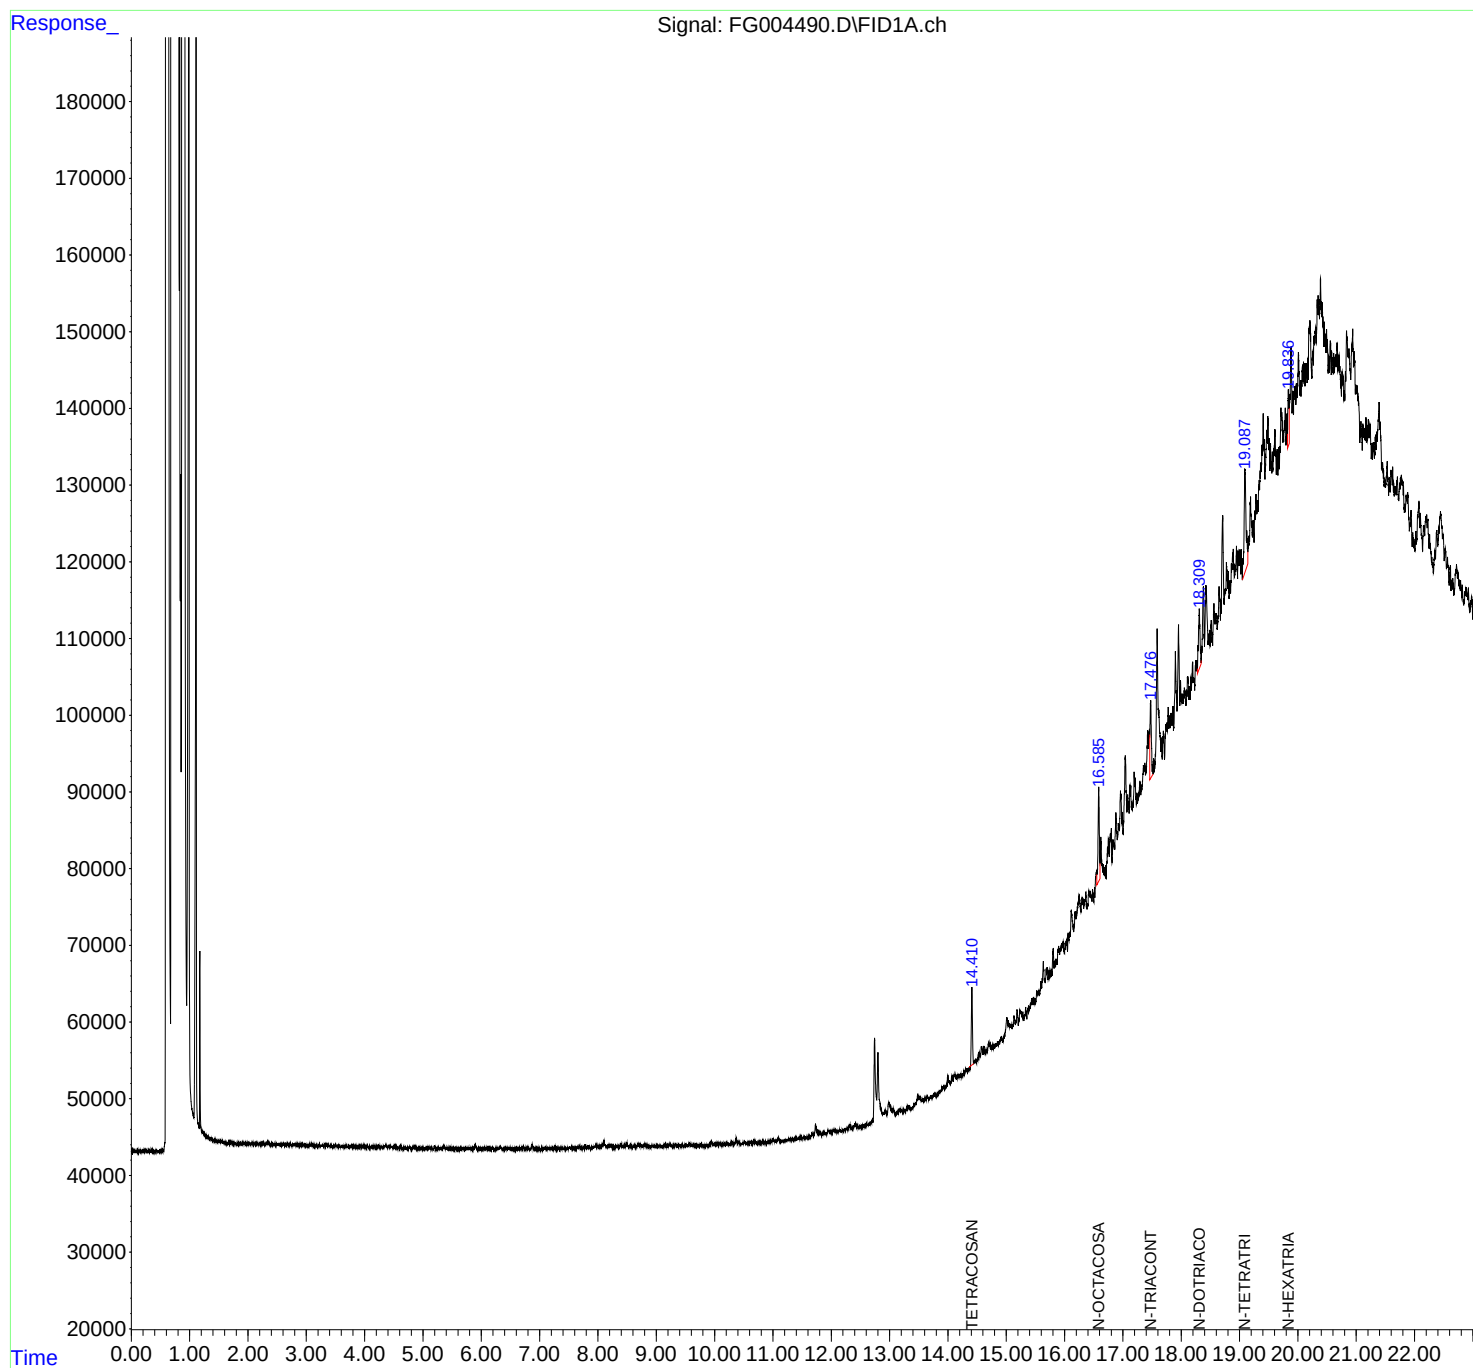


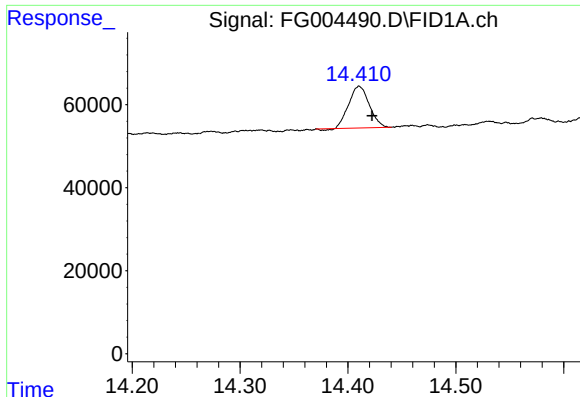

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.410 min
Delta R.T.: -0.012 min
Response: 132226
Conc: 1.28 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-C

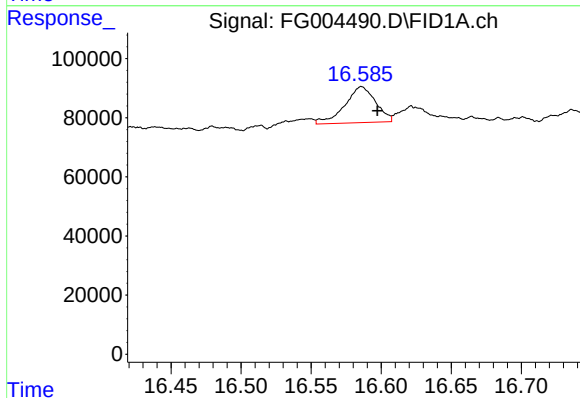


#12 N-OCTACOSANE

R.T.: 16.586 min
Delta R.T.: -0.011 min
Response: 186155
Conc: 1.61 ug/ml

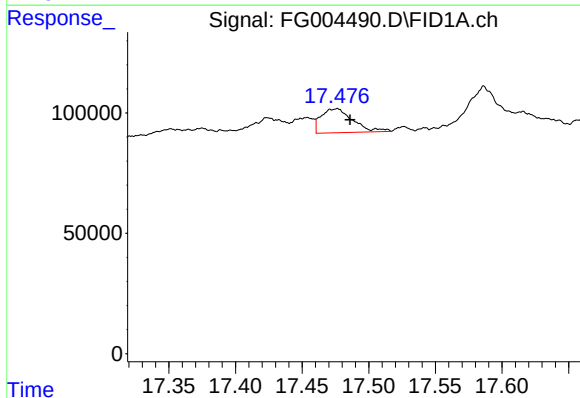


#13 N-TRIACONTANE

R.T.: 17.476 min
Delta R.T.: -0.010 min
Response: 165541
Conc: 1.40 ug/ml

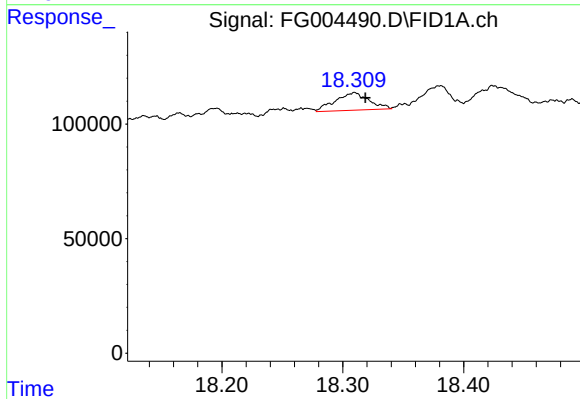

#14 N-DOTRIACONTANE


R.T.: 18.310 min
Delta R.T.: -0.009 min
Response: 148244
Conc: 1.26 ug/ml

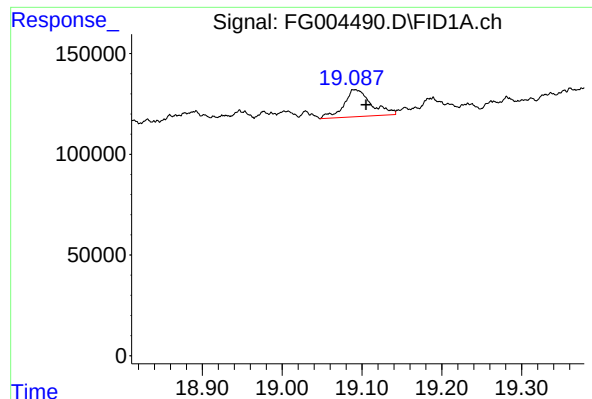

#15 N-TETRATRIACONTANE

R.T.: 19.091 min
Delta R.T.: -0.014 min
Response: 320961
Conc: 2.88 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-C

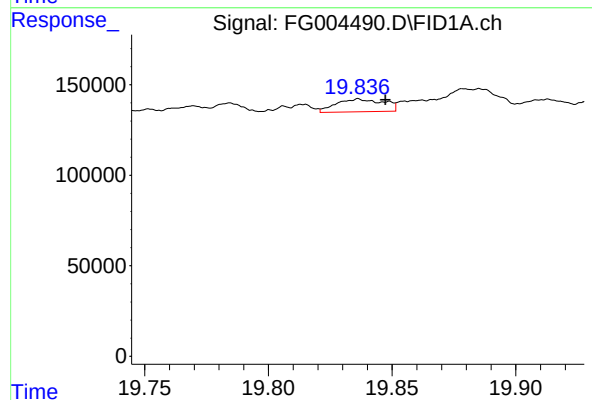

#16 N-HEXATRIACONTANE

R.T.: 19.836 min
Delta R.T.: -0.011 min
Response: 93512
Conc: 0.84 ug/ml