

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
 Data File : FG004492.D
 Signal(s) : FID1A.ch
 Acq On : 01 Apr 2019 17:02
 Operator : AJ\SJ
 Sample : K1689-03 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 NB-08-032919-A

Integration File: autoint1.e
 Quant Time: Apr 02 00:44:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.411	150222	1.456 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.637	141248	1.232 ug/ml
12) N-OCTACOSANE	16.586	371999	3.216 ug/ml
13) N-TRIACONTANE	17.479	570374	4.808 ug/ml
14) N-DOTRIACONTANE	18.309	295560	2.521 ug/ml
15) N-TETRATRIACONTANE	19.099	465034	4.174 ug/ml
16) N-HEXATRIACONTANE	19.846	359067	3.221 ug/ml
17) N-OCTATRIACONTANE	20.552	397615	4.000 ug/ml
18) N-TETRACONTANE	21.373	428516	3.962 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004492.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 17:02
Operator : AJ\SJ
Sample : K1689-03 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :
NB-08-032919-A

Integration File: autoint1.e
Quant Time: Apr 02 00:44:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

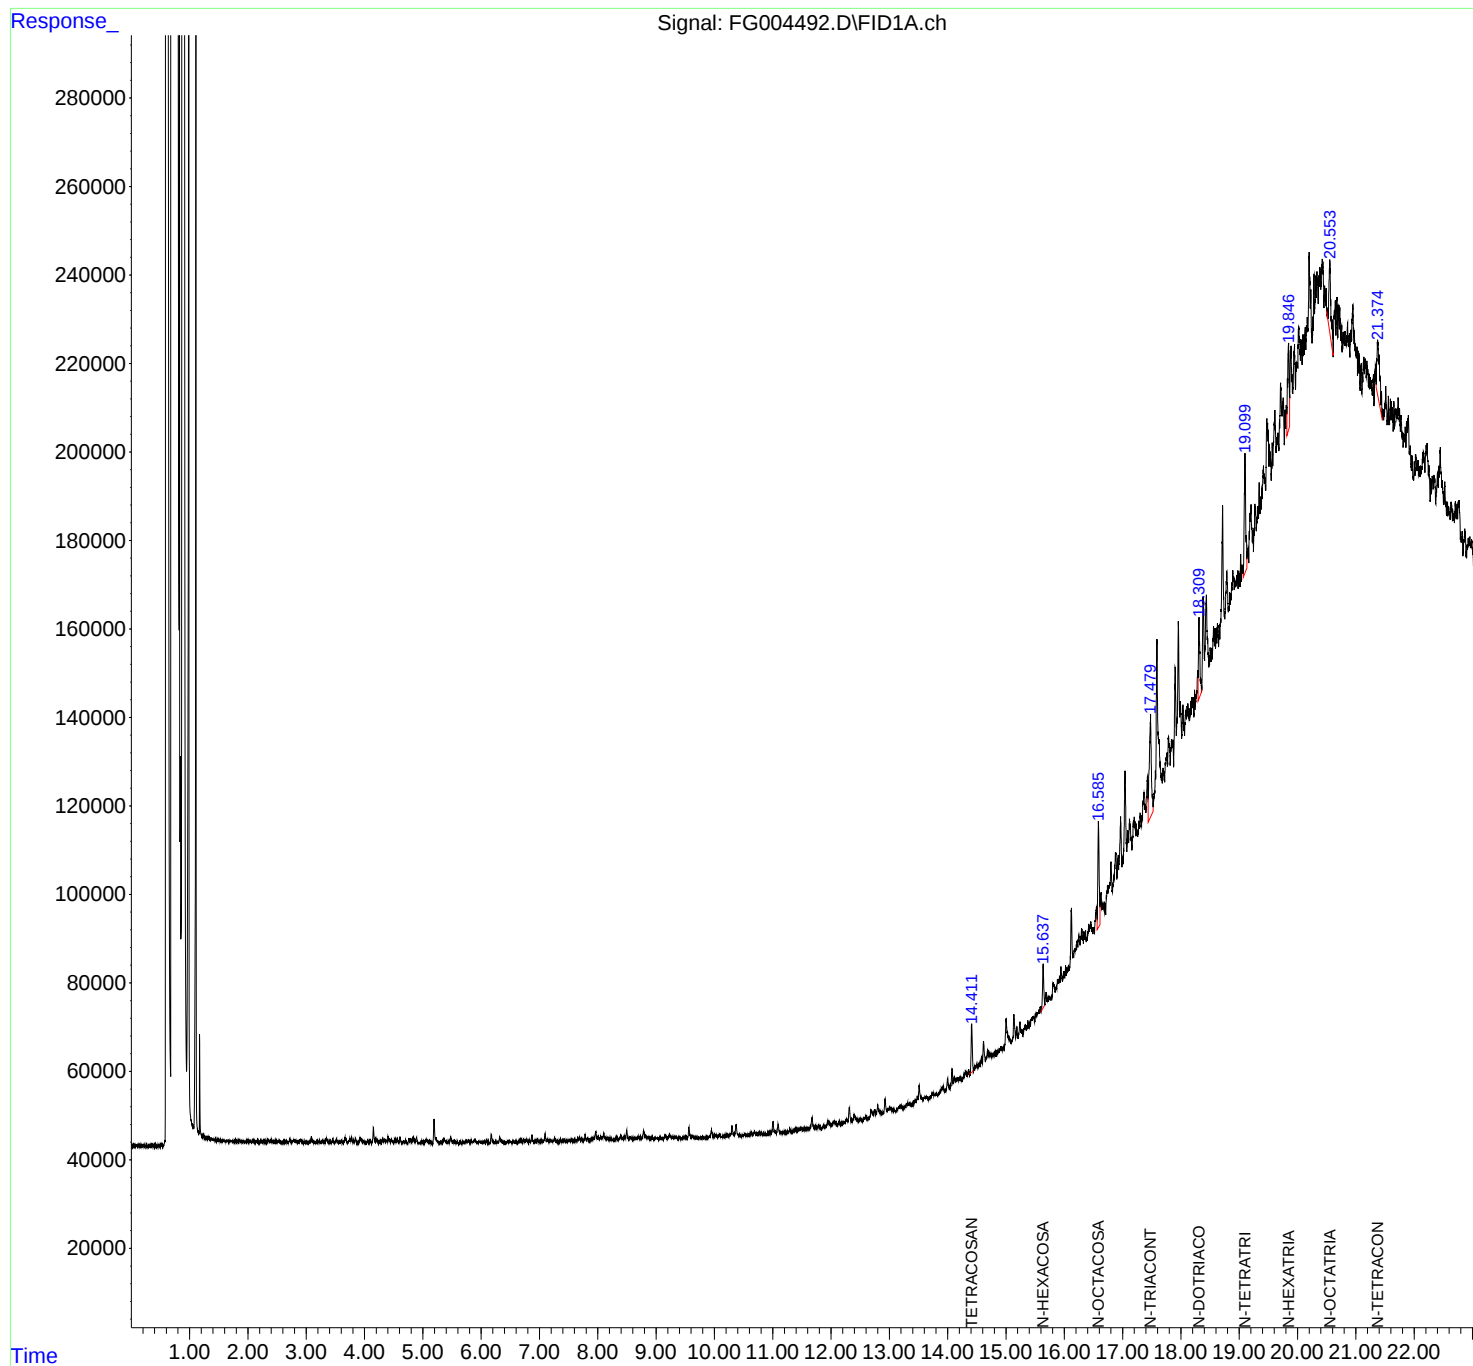


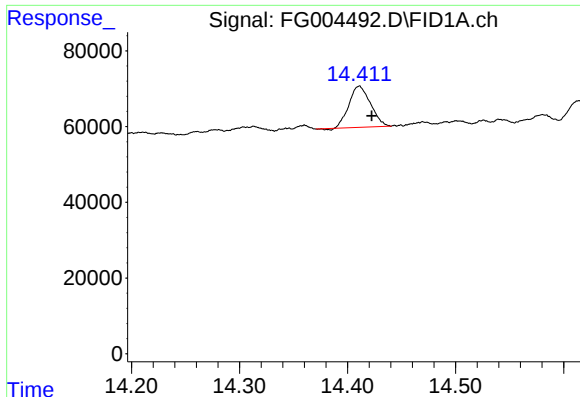

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.411 min
Delta R.T.: -0.012 min
Response: 150222
Conc: 1.46 ug/ml

Instrument :
FID_G
ClientSampleId :
NB-08-032919-A

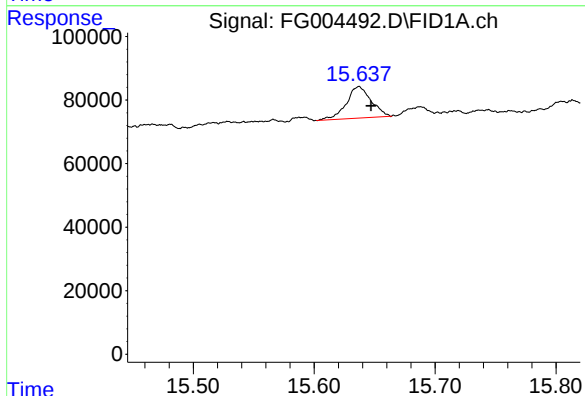


#11 N-HEXACOSANE

R.T.: 15.637 min
Delta R.T.: -0.010 min
Response: 141248
Conc: 1.23 ug/ml

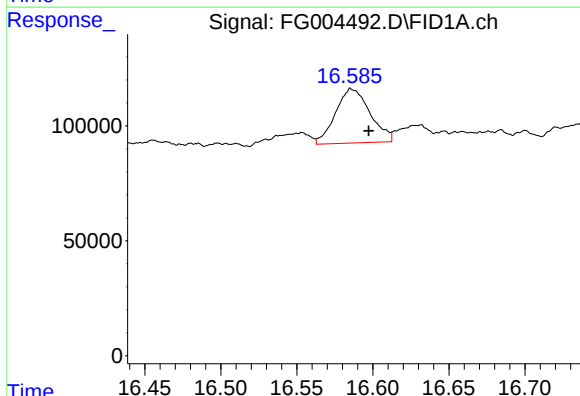


#12 N-OCTACOSANE

R.T.: 16.586 min
Delta R.T.: -0.011 min
Response: 371999
Conc: 3.22 ug/ml

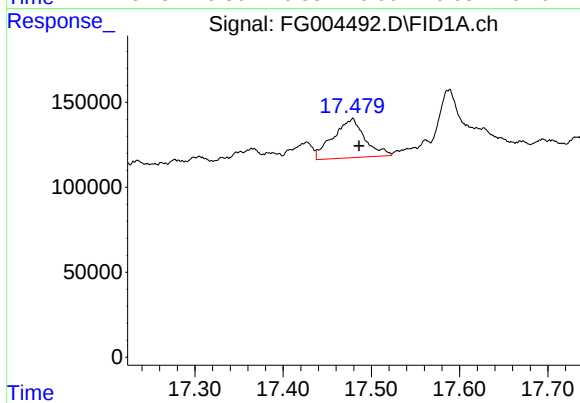

#13 N-TRIACONTANE


R.T.: 17.479 min
Delta R.T.: -0.007 min
Response: 570374
Conc: 4.81 ug/ml

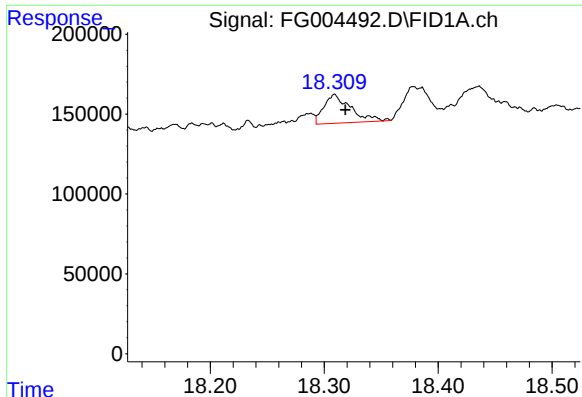

#14 N-DOTRIACONTANE


R.T.: 18.309 min
Delta R.T.: -0.009 min
Response: 295560
Conc: 2.52 ug/ml

Instrument :
FID_G
ClientSampleId :
NB-08-032919-A

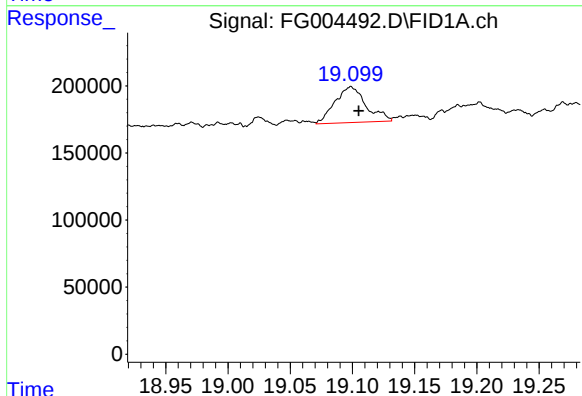


#15 N-TETRATRIACONTANE

R.T.: 19.099 min
Delta R.T.: -0.006 min
Response: 465034
Conc: 4.17 ug/ml

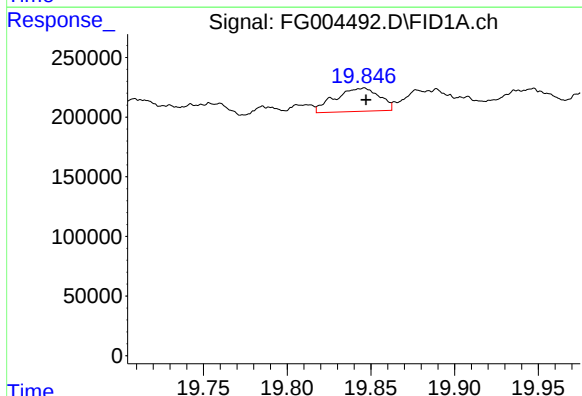


#16 N-HEXATRIACONTANE

R.T.: 19.846 min
Delta R.T.: -0.002 min
Response: 359067
Conc: 3.22 ug/ml

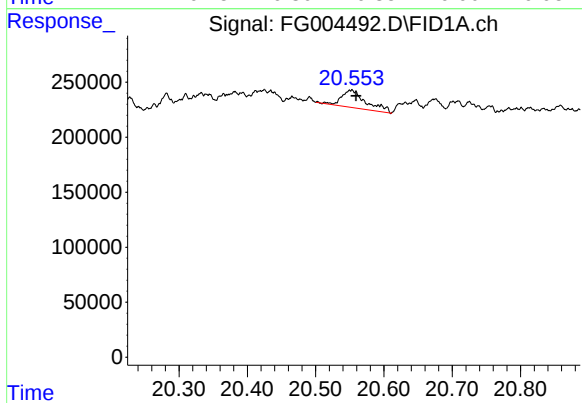

#17 N-OCTATRIACONTANE

R.T.: 20.552 min
Delta R.T.: -0.007 min
Response: 397615
Conc: 4.00 ug/ml

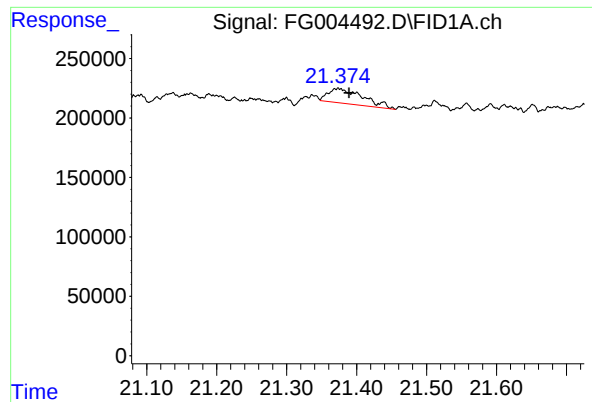

#18 N-TETRACONTANE

R.T.: 21.373 min
Delta R.T.: -0.016 min
Response: 428516
Conc: 3.96 ug/ml

Instrument :
FID_G
ClientSampleId :
NB-08-032919-A