

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004494.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 18:03
Operator : AJ\SJ
Sample : K1692-05 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-03-032919

Integration File: autoint1.e
Quant Time: Apr 02 00:45:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.368	1107630	9.689 ug/ml
10) N-TETRACOSANE	14.605	645810	5.591 ug/ml
12) N-OCTACOSANE	16.589	146718	1.268 ug/ml
13) N-TRIACONTANE	17.481	165466	1.395 ug/ml
14) N-DOTRIACONTANE	18.309	403699	3.443 ug/ml
15) N-TETRATRIACONTANE	19.102	142048	1.275 ug/ml
16) N-HEXATRIACONTANE	19.844	78008	0.700 ug/ml
17) N-OCTATRIACONTANE	20.628f	48127	0.484 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004494.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 18:03
Operator : AJ\SJ
Sample : K1692-05 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-03-032919

Integration File: autoint1.e
Quant Time: Apr 02 00:45:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

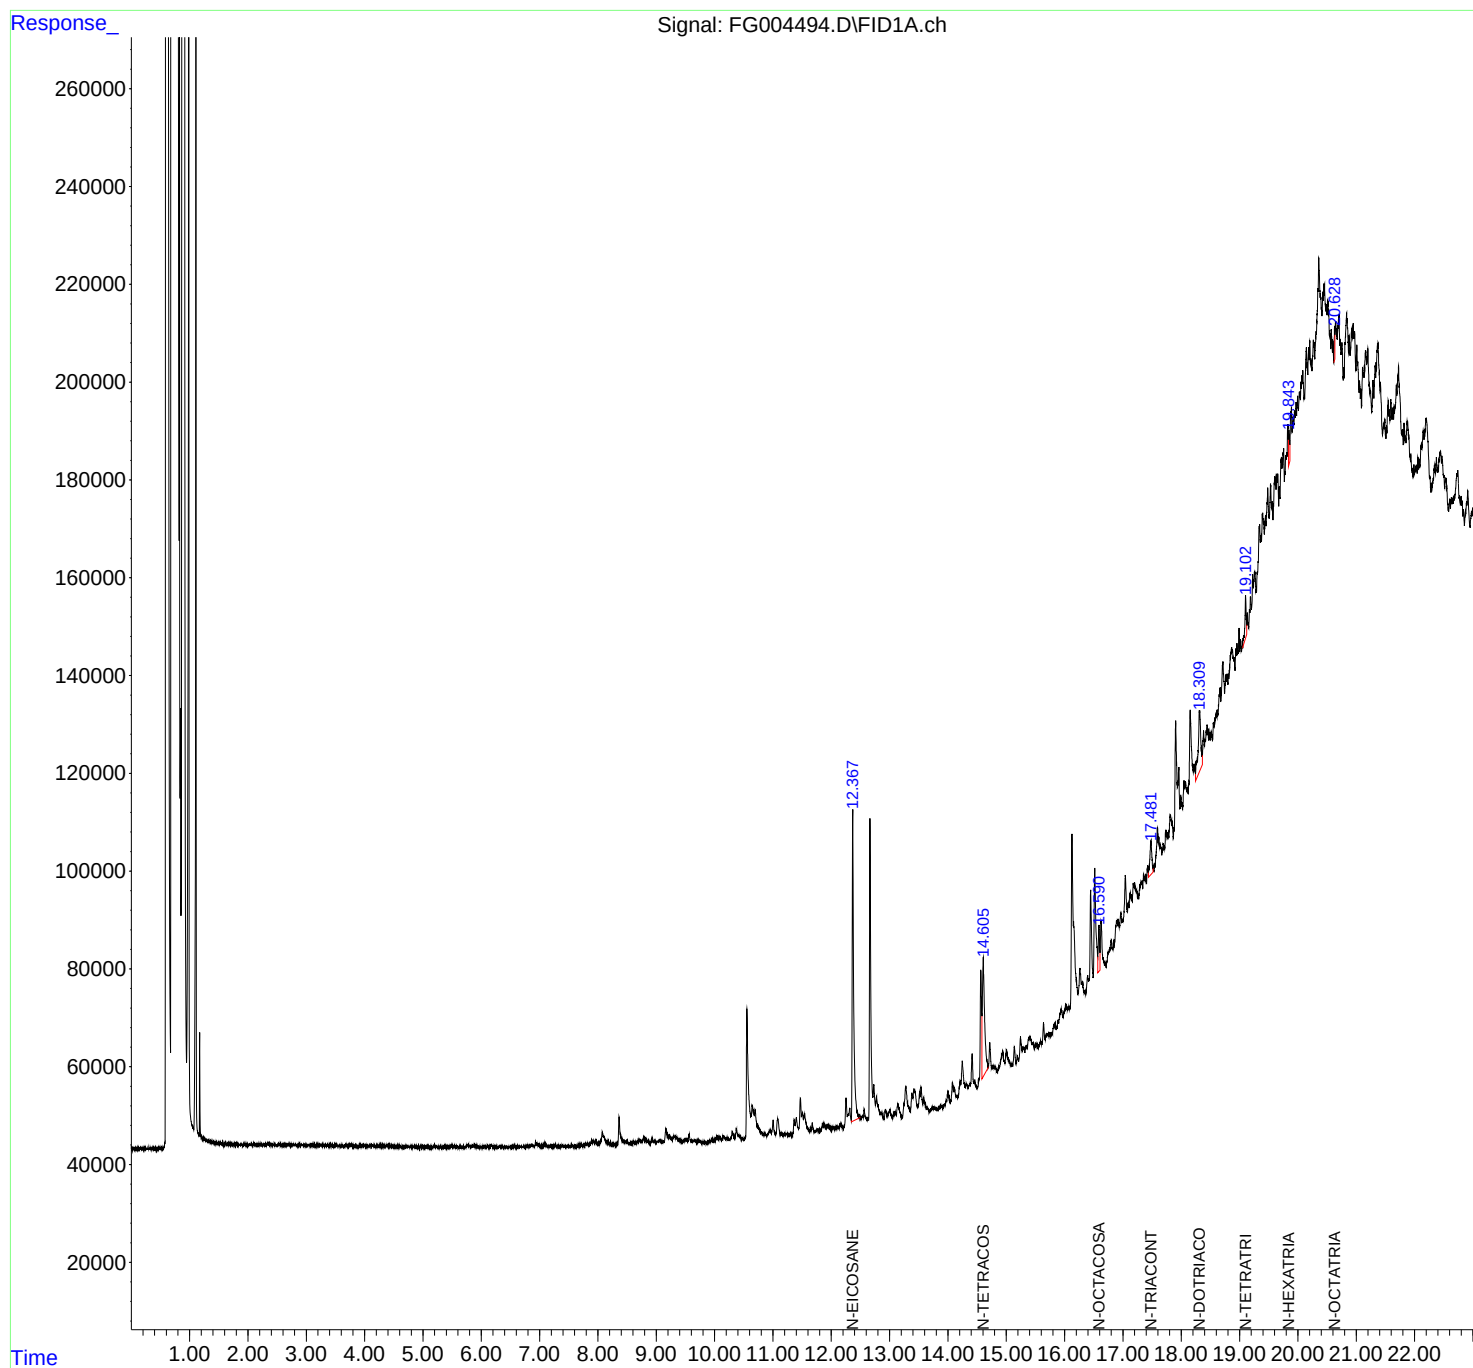


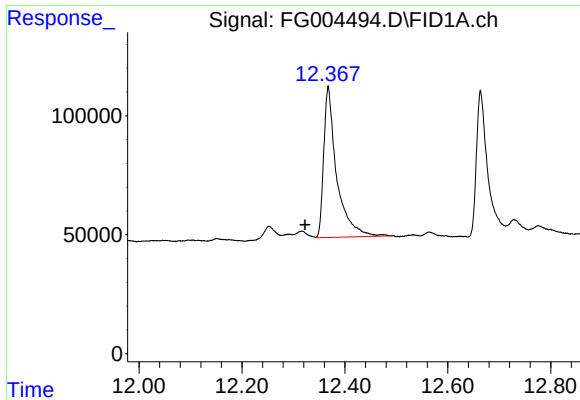

#7 N-EICOSANE


R.T.: 12.368 min
Delta R.T.: 0.045 min
Response: 1107630
Conc: 9.69 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-03-032919

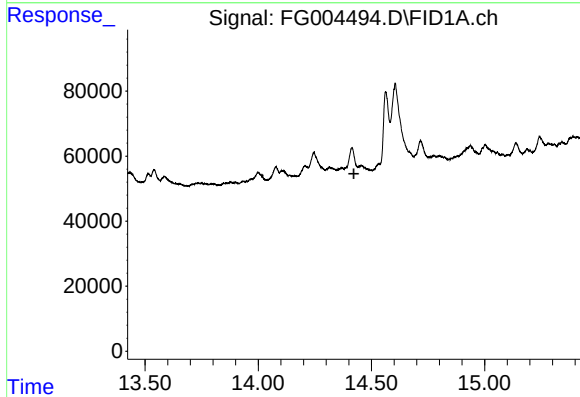


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

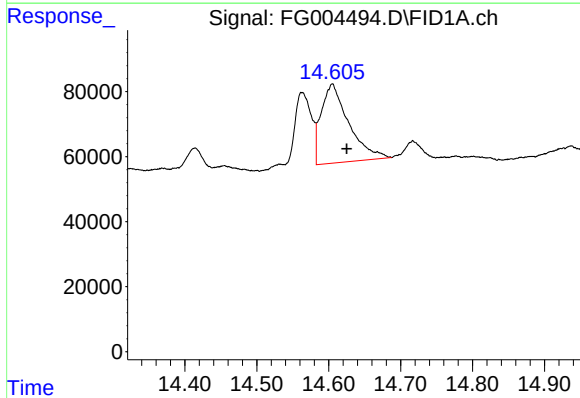


#10 N-TETRACOSANE

R.T.: 14.605 min
Delta R.T.: -0.020 min
Response: 645810
Conc: 5.59 ug/ml

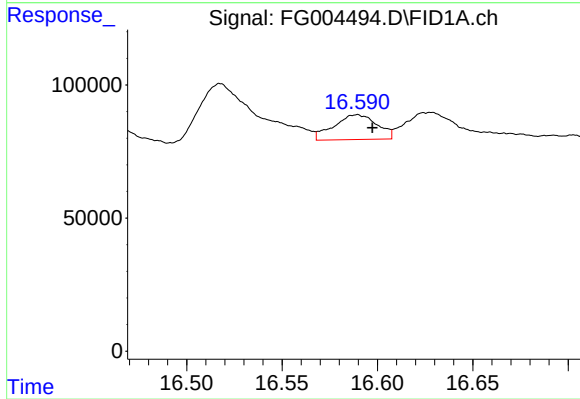

#12 N-OCTACOSANE


R.T.: 16.589 min
Delta R.T.: -0.008 min
Response: 146718
Conc: 1.27 ug/ml

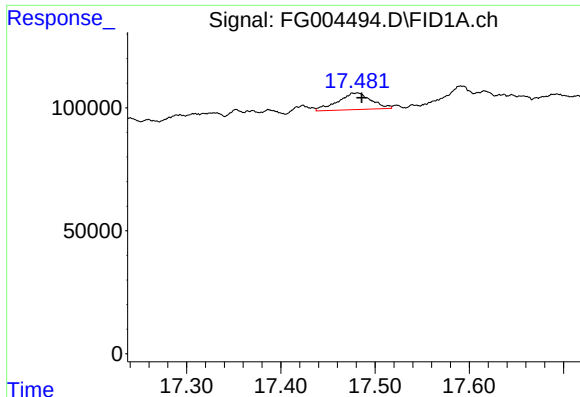

#13 N-TRIACONTANE


R.T.: 17.481 min
Delta R.T.: -0.005 min
Response: 165466
Conc: 1.39 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-03-032919

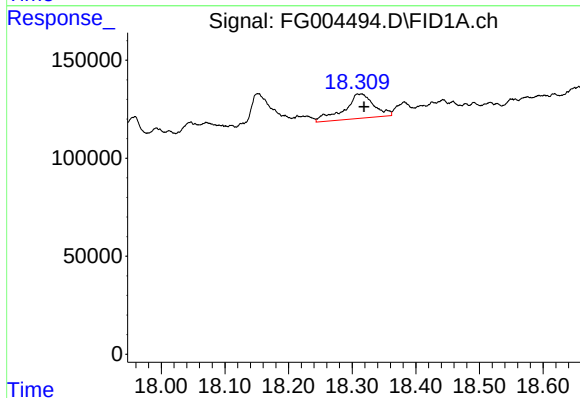


#14 N-DOTRIACONTANE

R.T.: 18.309 min
Delta R.T.: -0.010 min
Response: 403699
Conc: 3.44 ug/ml

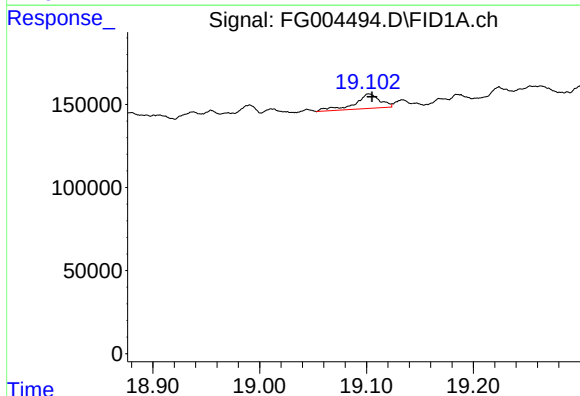


#15 N-TETRATRIACONTANE

R.T.: 19.102 min
Delta R.T.: -0.003 min
Response: 142048
Conc: 1.27 ug/ml

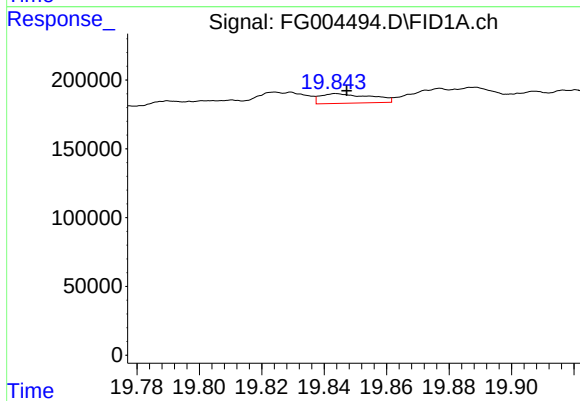

#16 N-HEXATRIACONTANE

R.T.: 19.844 min
Delta R.T.: -0.003 min
Response: 78008
Conc: 0.70 ug/ml

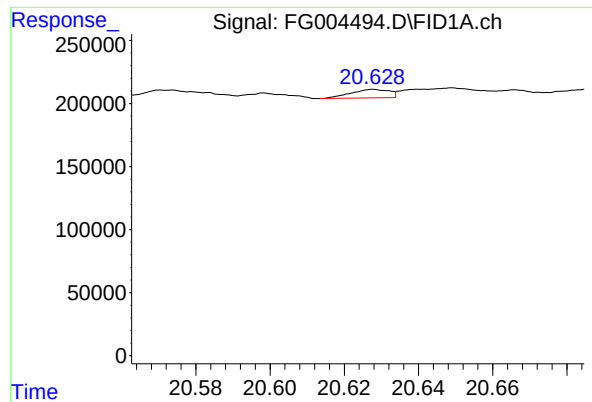

#17 N-OCTATRIACONTANE

R.T.: 20.628 min
Delta R.T.: 0.069 min
Response: 48127
Conc: 0.48 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-03-032919