

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004504.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 23:07
Operator : AJ\SJ
Sample : K2056-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CS-10

Integration File: autoint1.e
Quant Time: Apr 02 00:48:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.412	1616595	15.673 ug/ml
Target Compounds			
4) N-TETRADECANE	8.032f	54517	0.503 ug/ml
7) N-EICOSANE	12.362	2046368	17.901 ug/ml
10) N-TETRACOSANE	14.594	926650	8.022 ug/ml
12) N-OCTACOSANE	16.587	135208	1.169 ug/ml
13) N-TRIACONTANE	17.473	133923	1.129 ug/ml
14) N-DOTRIACONTANE	18.304	223397	1.905 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004504.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 23:07
Operator : AJ\SJ
Sample : K2056-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CS-10

Integration File: autoint1.e
Quant Time: Apr 02 00:48:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

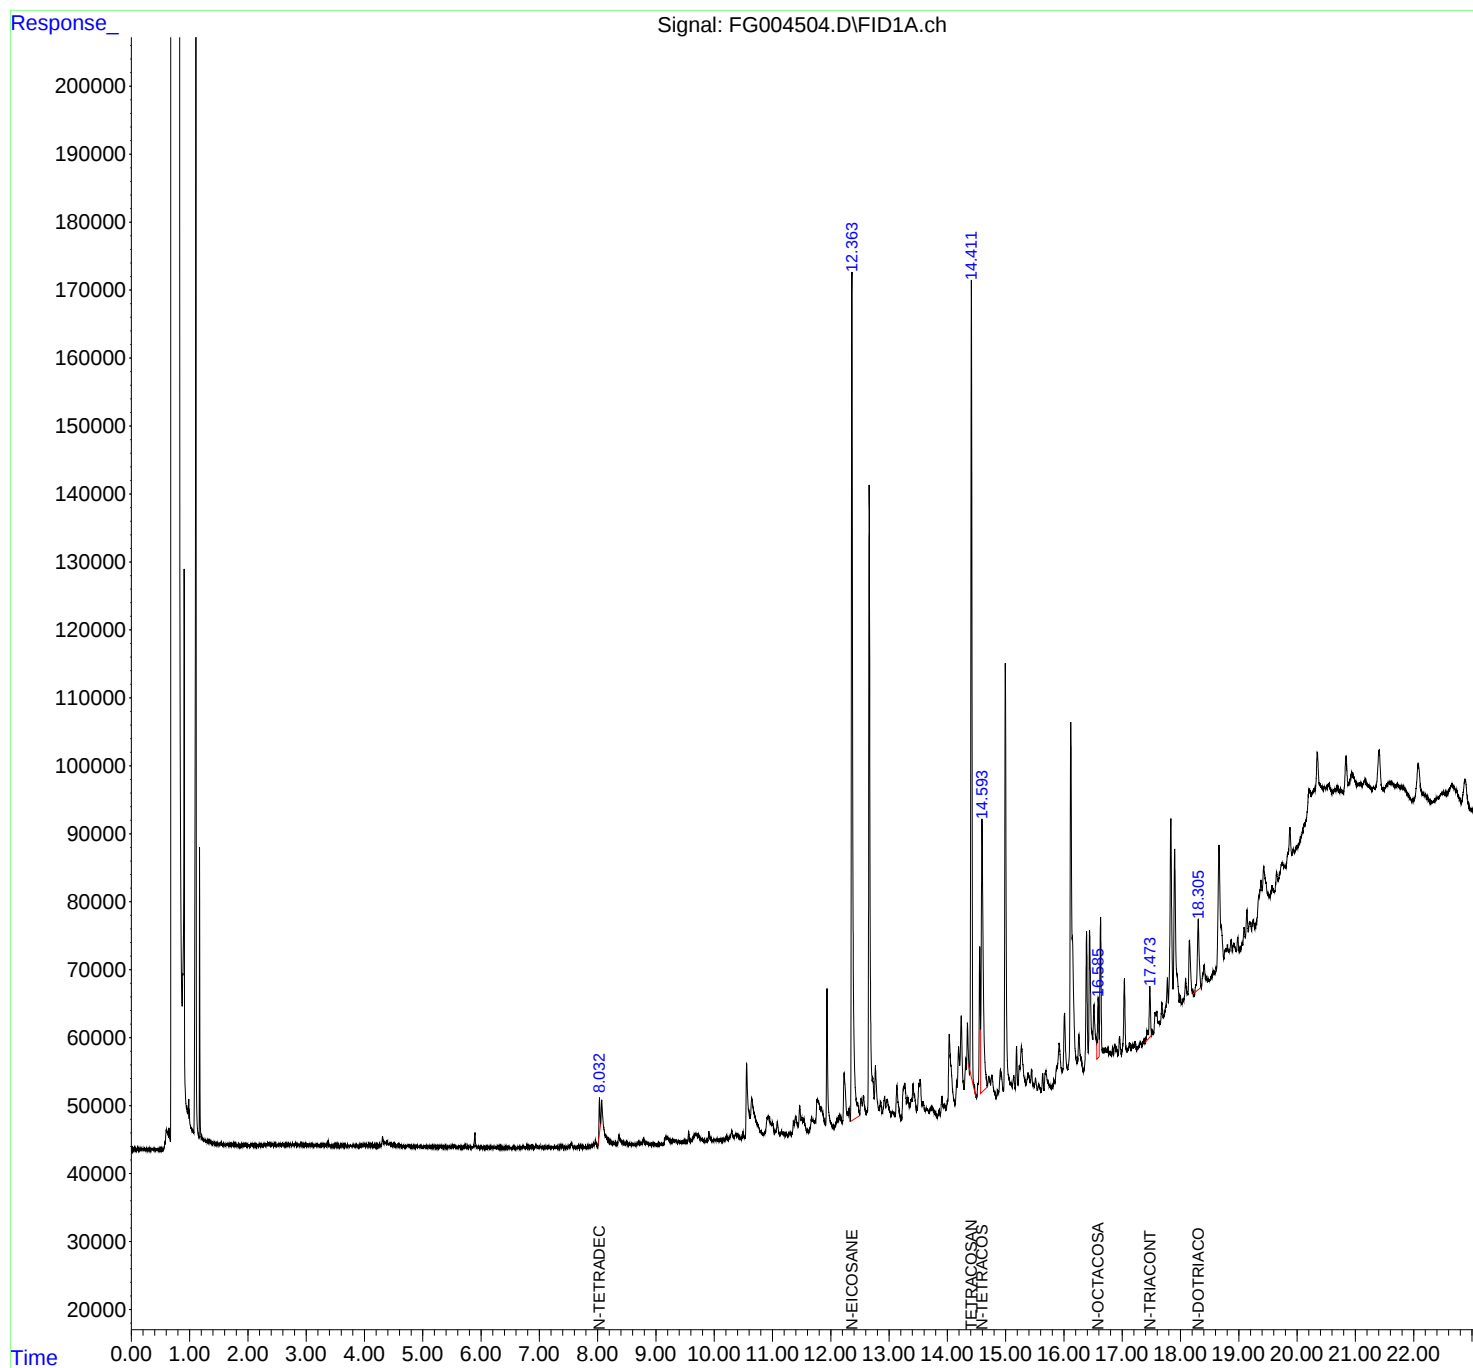


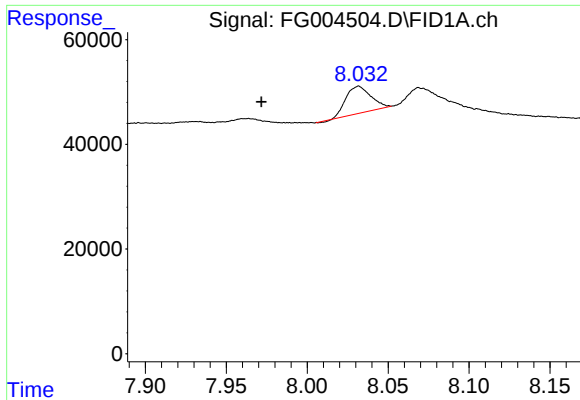

#4 N-TETRADECANE


R.T.: 8.032 min
Delta R.T.: 0.060 min
Response: 54517
Conc: 0.50 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-10

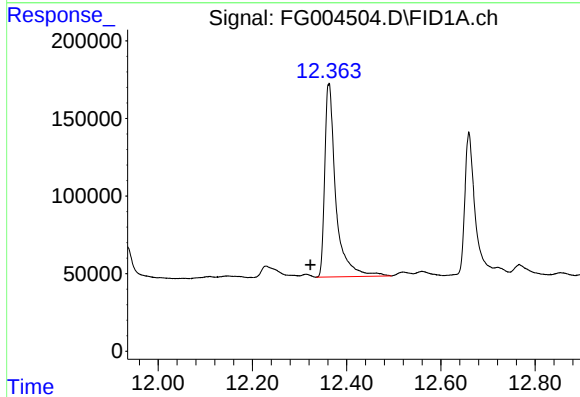


#7 N-EICOSANE

R.T.: 12.362 min
Delta R.T.: 0.039 min
Response: 2046368
Conc: 17.90 ug/ml

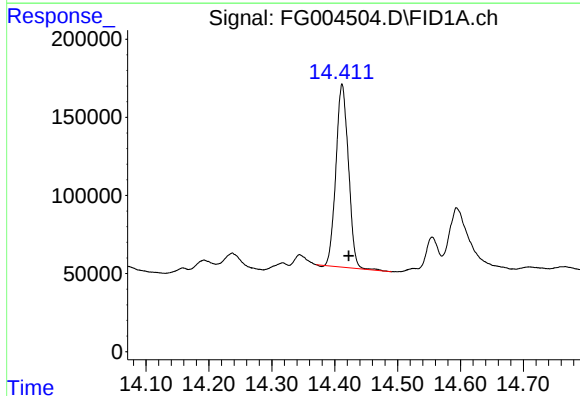


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.412 min
Delta R.T.: -0.011 min
Response: 1616595
Conc: 15.67 ug/ml

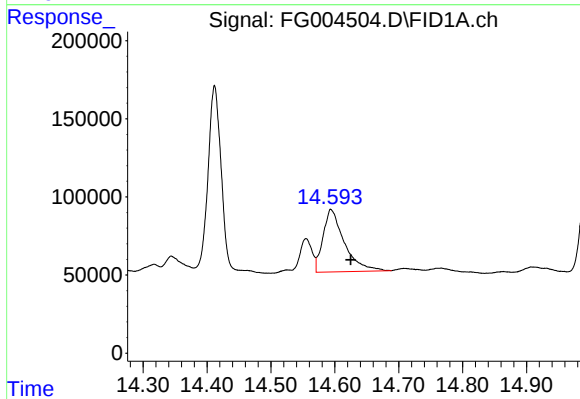

#10 N-TETRACOSANE


R.T.: 14.594 min
Delta R.T.: -0.031 min
Response: 926650
Conc: 8.02 ug/ml

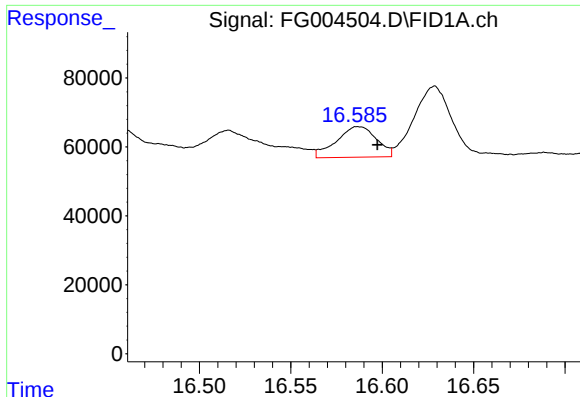

#12 N-OCTACOSANE


R.T.: 16.587 min
Delta R.T.: -0.010 min
Response: 135208
Conc: 1.17 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-10

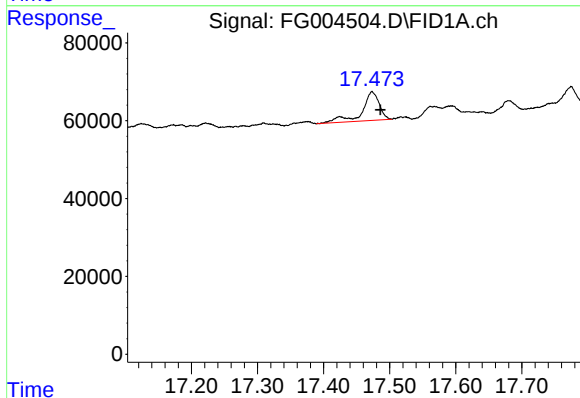

#13 N-TRIACONTANE

R.T.: 17.473 min
Delta R.T.: -0.013 min
Response: 133923
Conc: 1.13 ug/ml

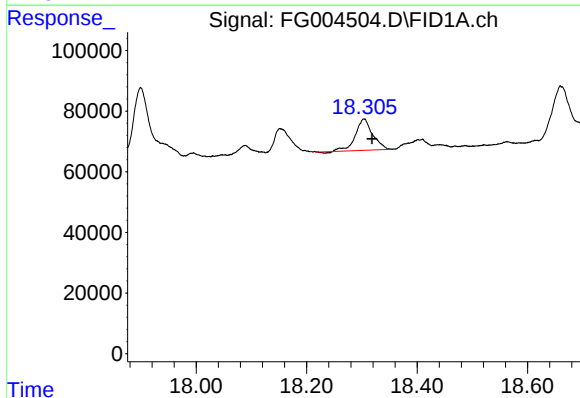

#14 N-DOTRIACONTANE

R.T.: 18.304 min
Delta R.T.: -0.015 min
Response: 223397
Conc: 1.91 ug/ml