

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004508.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 01:08
Operator : AJ\SJ
Sample : K1685-11 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

Integration File: autoint1.e
Quant Time: Apr 02 05:30:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

8)	N-DOCOSANE	13.563	200624	1.755 ug/ml
10)	N-TETRACOSANE	14.617	299818	2.595 ug/ml
12)	N-OCTACOSANE	16.585	98311	0.850 ug/ml
13)	N-TRIACONTANE	17.474	114465	0.965 ug/ml
14)	N-DOTRIACONTANE	18.308	151989	1.296 ug/ml
15)	N-TETRATRIACONTANE	19.093	96307	0.864 ug/ml
16)	N-HEXATRIACONTANE	19.833	82579	0.741 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004508.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 01:08
Operator : AJ\SJ
Sample : K1685-11 20X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

Integration File: autoint1.e
Quant Time: Apr 02 05:30:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

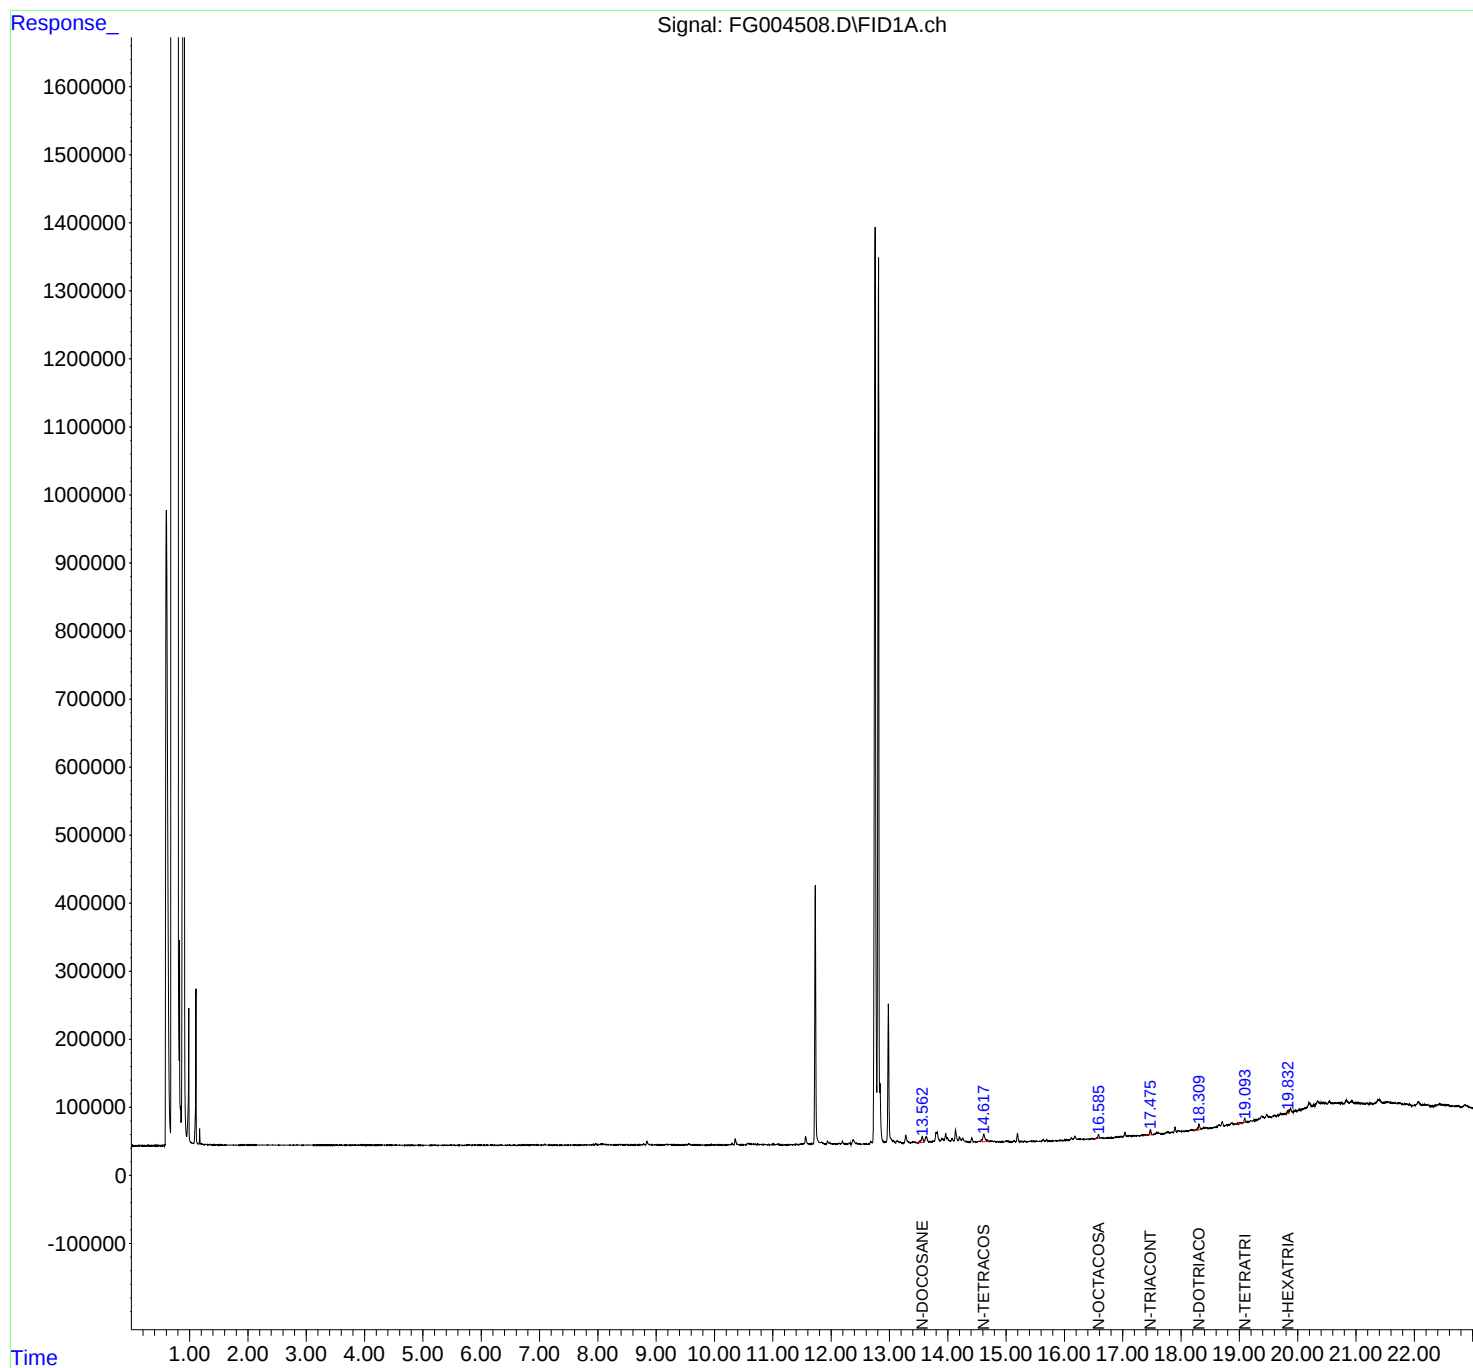


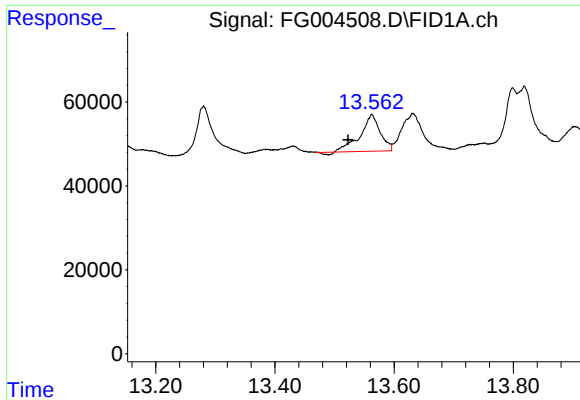

#8 N-DOCOSANE


R.T.: 13.563 min
Delta R.T.: 0.040 min
Response: 200624
Conc: 1.76 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

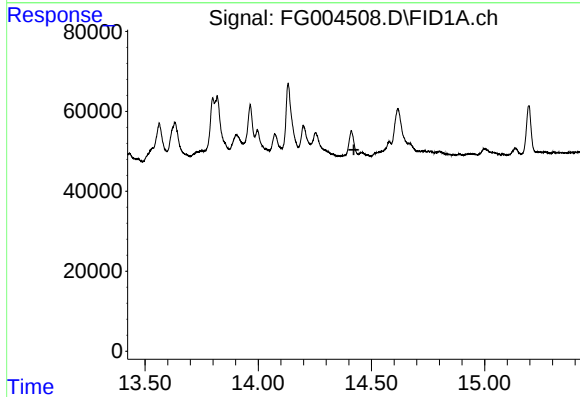


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

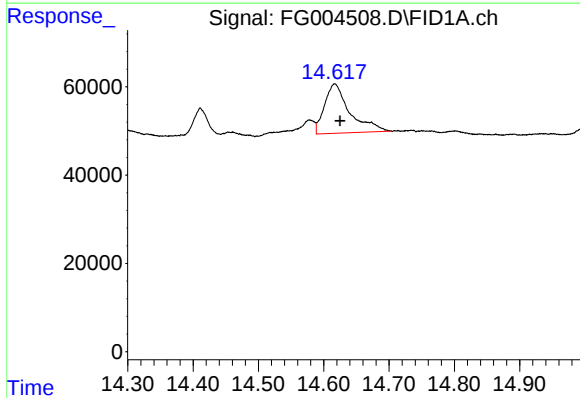


#10 N-TETRACOSANE

R.T.: 14.617 min
Delta R.T.: -0.008 min
Response: 299818
Conc: 2.60 ug/ml

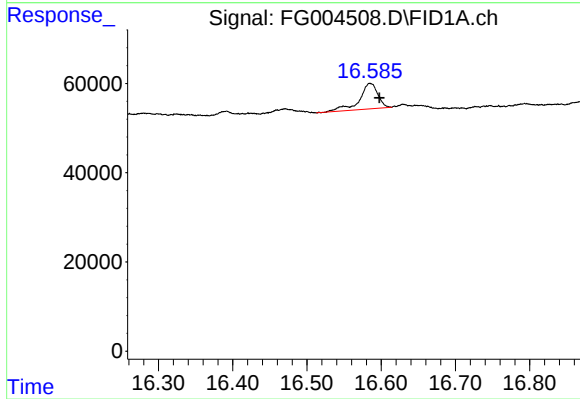

#12 N-OCTACOSANE


R.T.: 16.585 min
Delta R.T.: -0.012 min
Response: 98311
Conc: 0.85 ug/ml

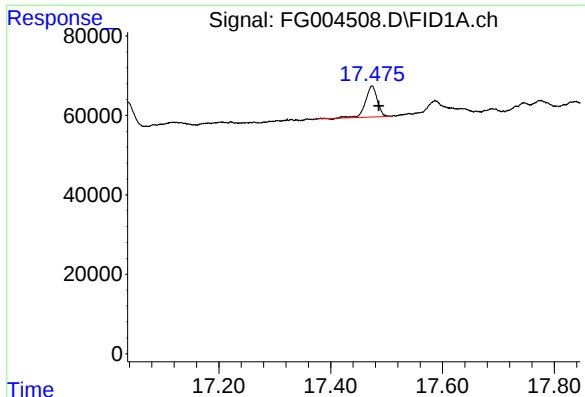

#13 N-TRIACONTANE


R.T.: 17.474 min
Delta R.T.: -0.012 min
Response: 114465
Conc: 0.96 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-B

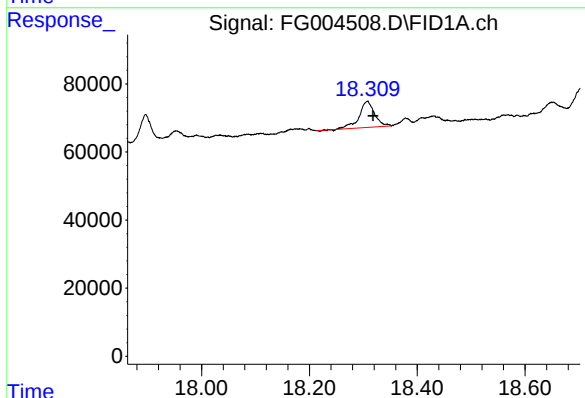


#14 N-DOTRIACONTANE

R.T.: 18.308 min
Delta R.T.: -0.011 min
Response: 151989
Conc: 1.30 ug/ml

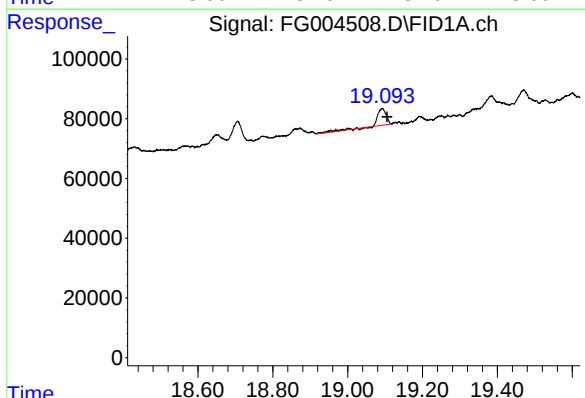

#15 N-TETRATRIACONTANE

R.T.: 19.093 min
Delta R.T.: -0.012 min
Response: 96307
Conc: 0.86 ug/ml

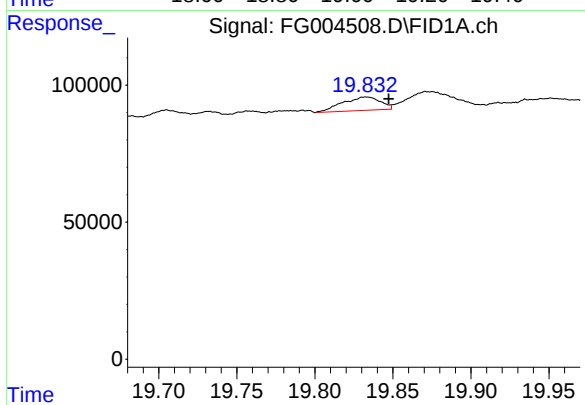

#16 N-HEXATRIACONTANE

R.T.: 19.833 min
Delta R.T.: -0.014 min
Response: 82579
Conc: 0.74 ug/ml