

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
 Data File : FG004509.D
 Signal(s) : FID1A.ch
 Acq On : 02 Apr 2019 01:38
 Operator : AJ\SJ
 Sample : K1685-13 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 AU-06-032819-C

Integration File: autoint1.e
 Quant Time: Apr 02 05:30:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.411	259468	2.516 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.588	294682	2.547 ug/ml
13) N-TRIACONTANE	17.480	180630	1.523 ug/ml
14) N-DOTRIACONTANE	18.305	265687	2.266 ug/ml
15) N-TETRATRIACONTANE	19.093	331722	2.977 ug/ml
16) N-HEXATRIACONTANE	19.843	101726	0.913 ug/ml
17) N-OCTATRIACONTANE	20.540	40860	0.411 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004509.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 01:38
Operator : AJ\SJ
Sample : K1685-13 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :
AU-06-032819-C

Integration File: autoint1.e
Quant Time: Apr 02 05:30:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

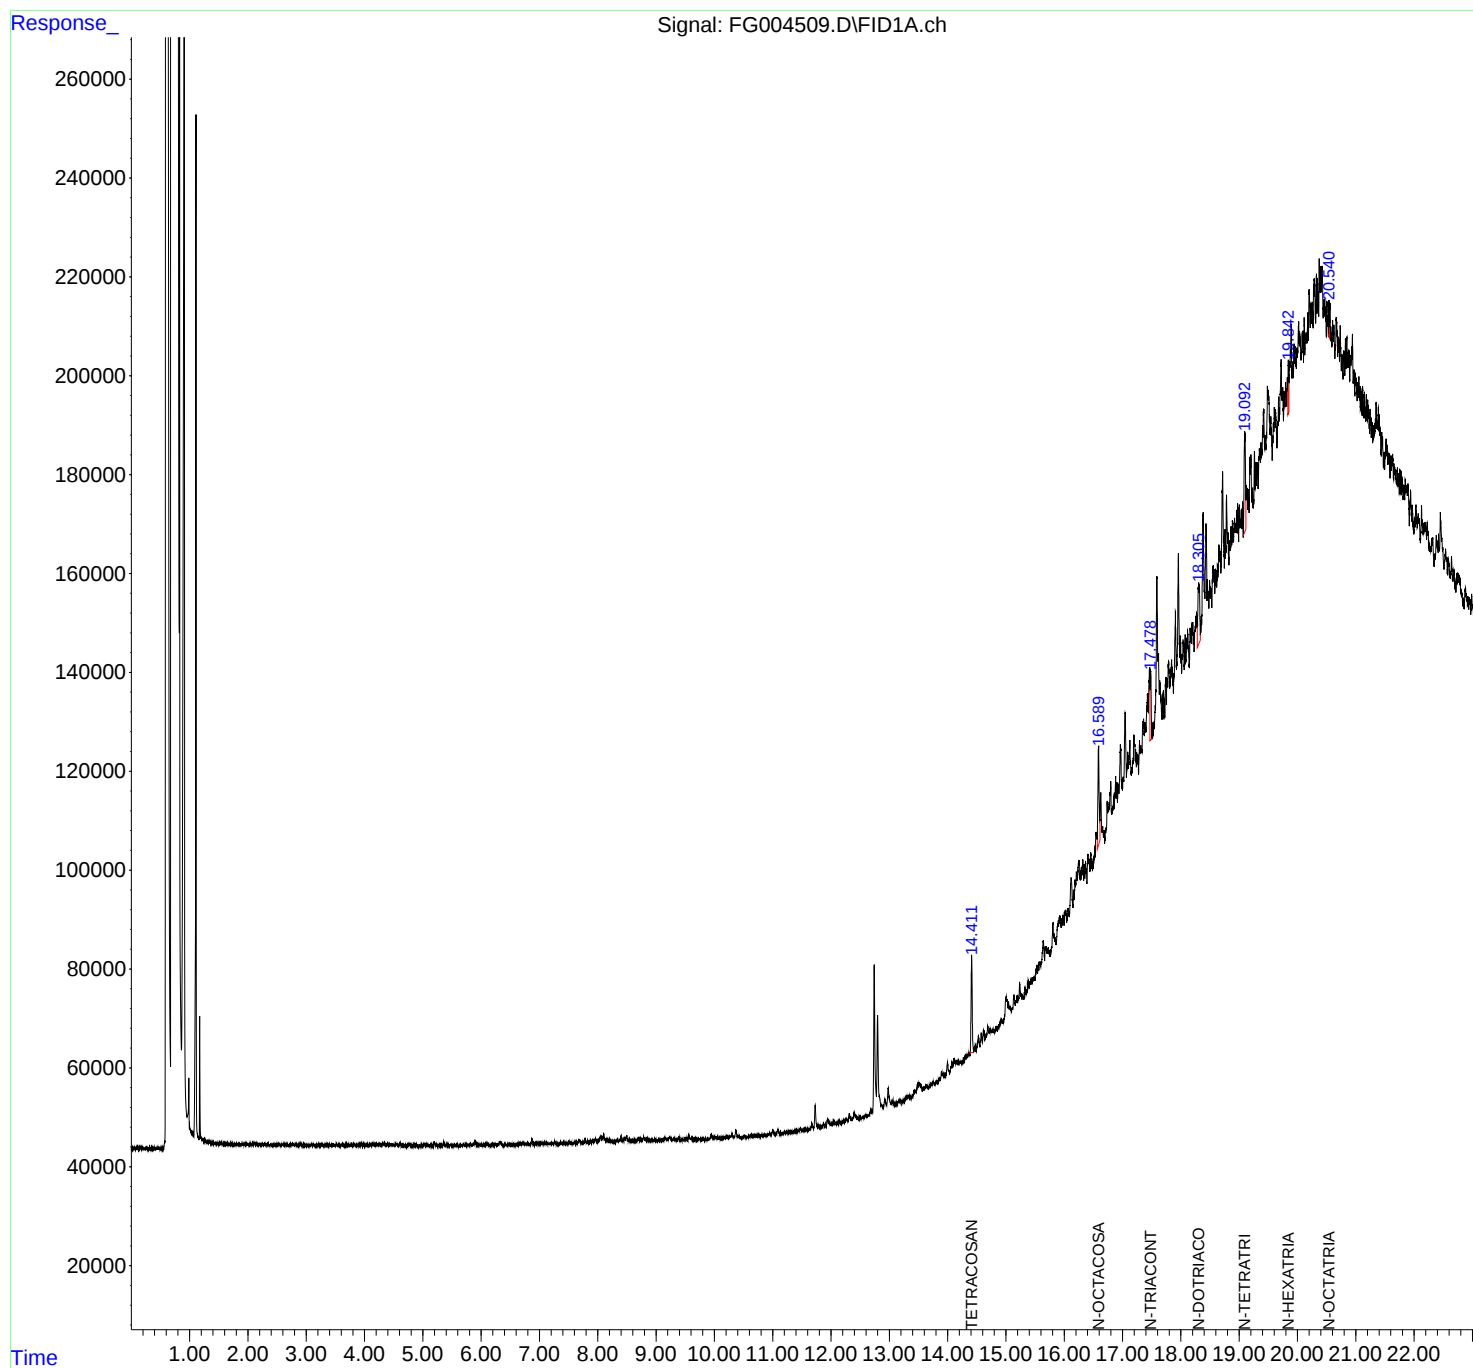


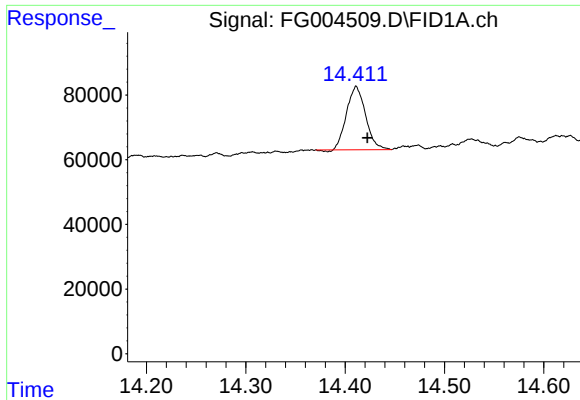

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.411 min
Delta R.T.: -0.011 min
Response: 259468
Conc: 2.52 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-C

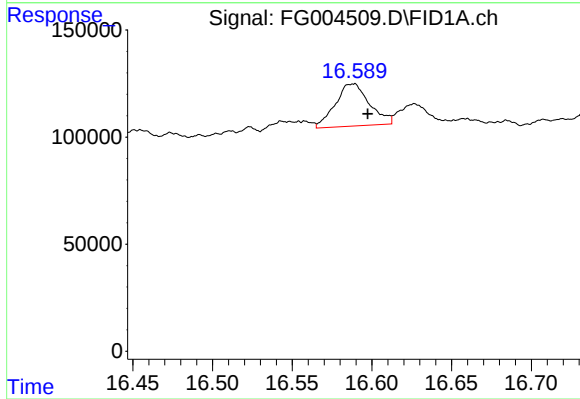


#12 N-OCTACOSANE

R.T.: 16.588 min
Delta R.T.: -0.009 min
Response: 294682
Conc: 2.55 ug/ml

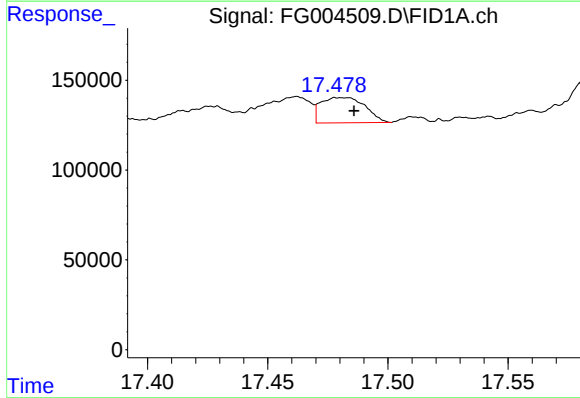


#13 N-TRIACONTANE

R.T.: 17.480 min
Delta R.T.: -0.006 min
Response: 180630
Conc: 1.52 ug/ml

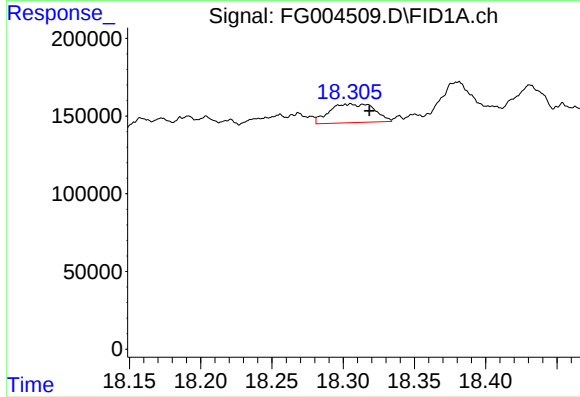

#14 N-DOTRIACONTANE


R.T.: 18.305 min
Delta R.T.: -0.013 min
Response: 265687
Conc: 2.27 ug/ml

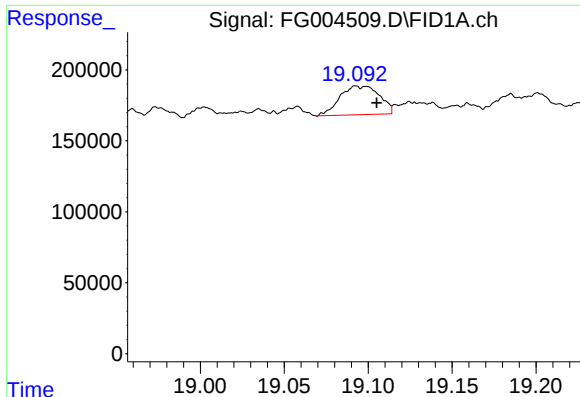

#15 N-TETRATRIACONTANE


R.T.: 19.093 min
Delta R.T.: -0.012 min
Response: 331722
Conc: 2.98 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-032819-C

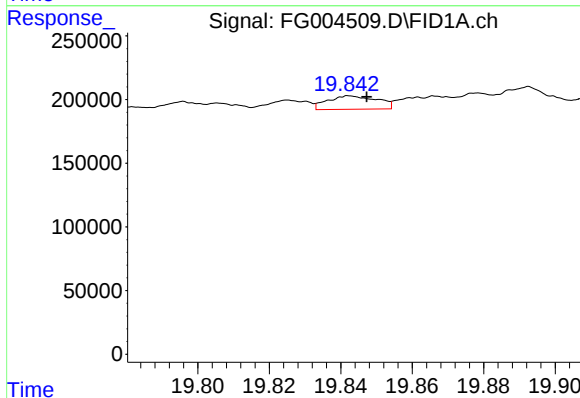

#16 N-HEXATRIACONTANE

R.T.: 19.843 min
Delta R.T.: -0.005 min
Response: 101726
Conc: 0.91 ug/ml

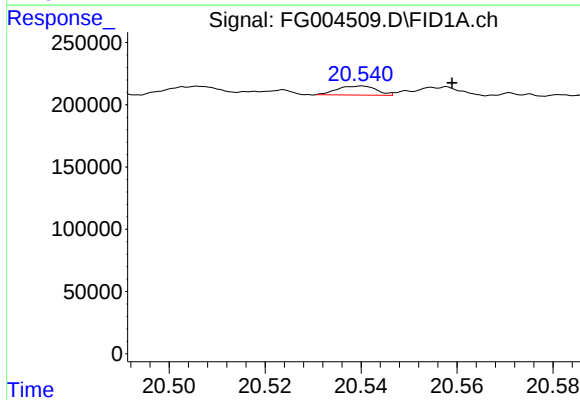

#17 N-OCTATRIACONTANE

R.T.: 20.540 min
Delta R.T.: -0.019 min
Response: 40860
Conc: 0.41 ug/ml