

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004511.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 02:38
Operator : AJ\SJ
Sample : K1698-03 20X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TR-05-032819

Integration File: autoint1.e
Quant Time: Apr 02 05:30:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

7)	N-EICOSANE	12.375f	192252	1.682 ug/ml
10)	N-TETRACOSANE	14.617	197980	1.714 ug/ml
11)	N-HEXACOSANE	15.638	100958	0.881 ug/ml
12)	N-OCTACOSANE	16.589	179978	1.556 ug/ml
13)	N-TRIACONTANE	17.478	220067	1.855 ug/ml
14)	N-DOTRIACONTANE	18.312	198030	1.689 ug/ml
15)	N-TETRATRIACONTANE	19.094	198052	1.778 ug/ml
16)	N-HEXATRIACONTANE	19.842	106281	0.953 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004511.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 02:38
Operator : AJ\SJ
Sample : K1698-03 20X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TR-05-032819

Integration File: autoint1.e
Quant Time: Apr 02 05:30:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

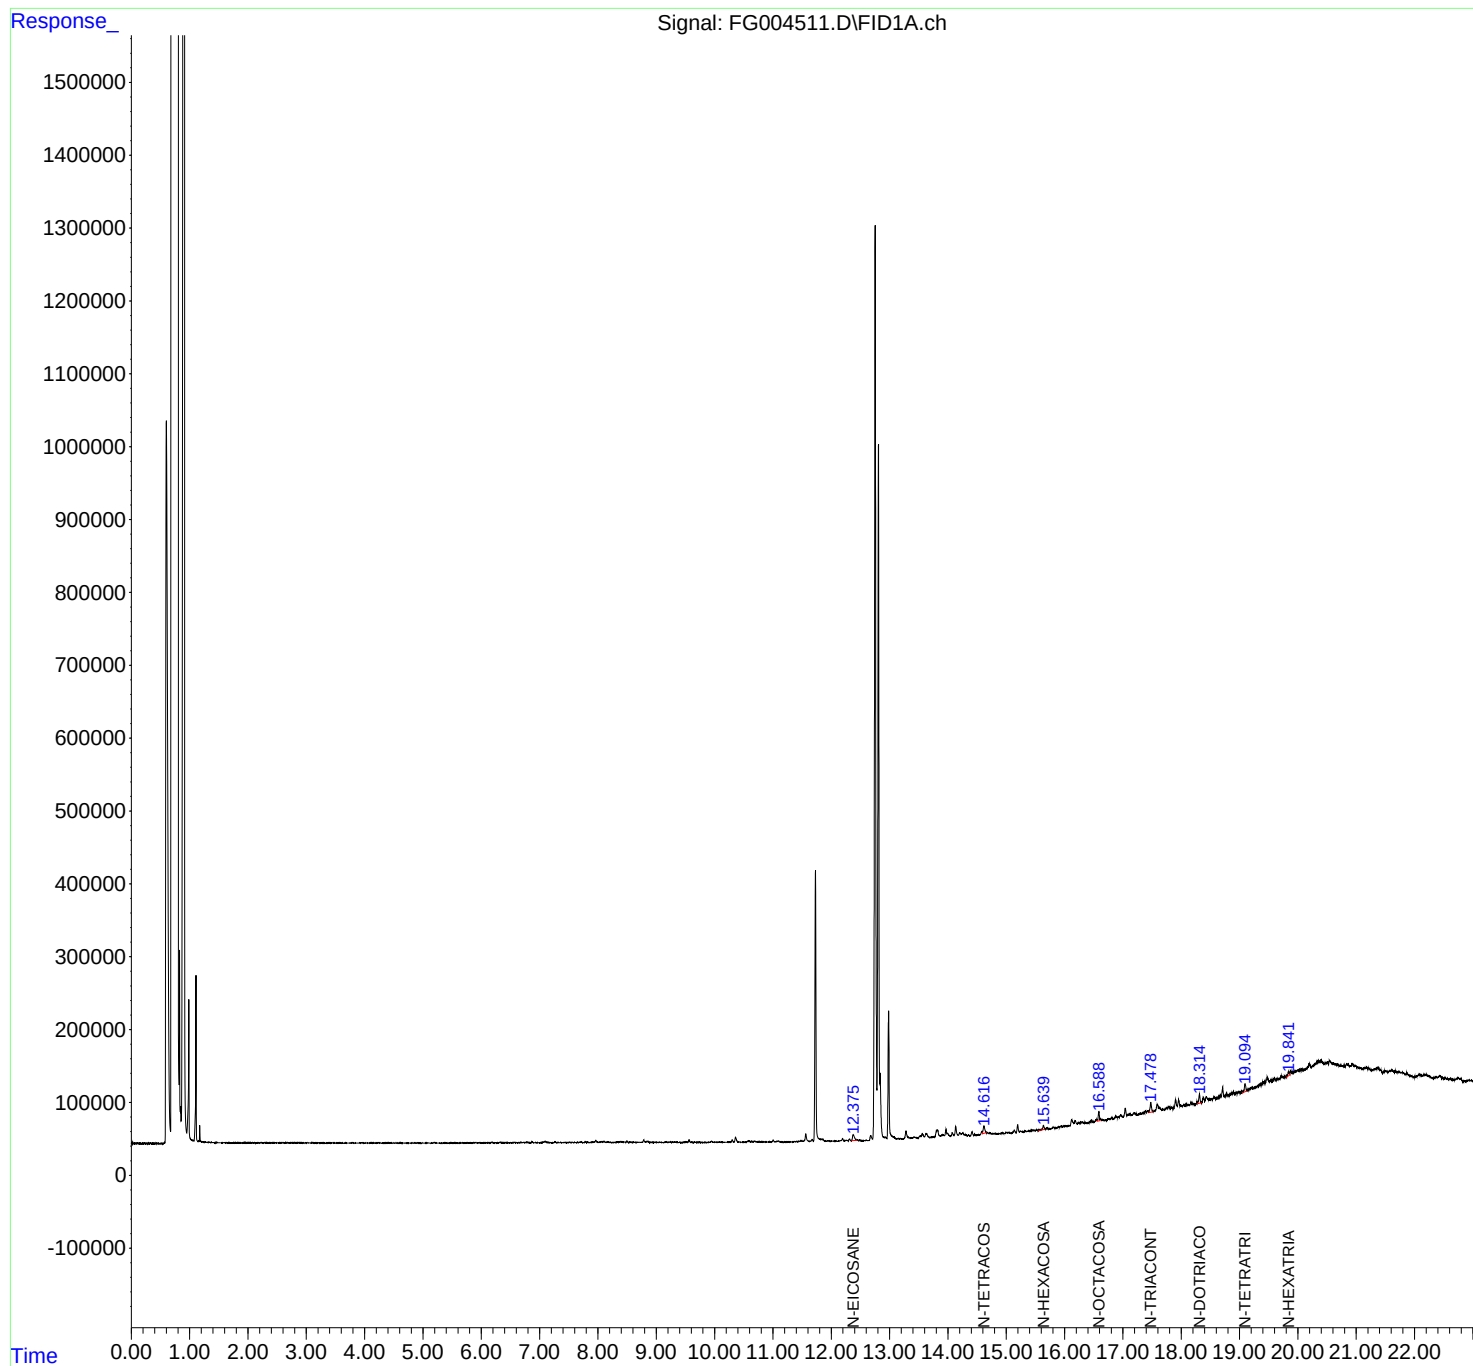


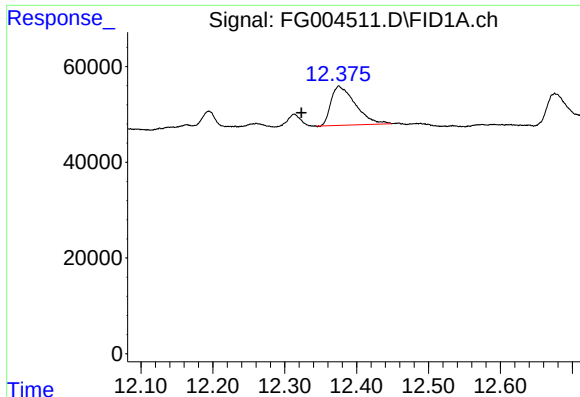

#7 N-EICOSANE


R.T.: 12.375 min
Delta R.T.: 0.052 min
Response: 192252
Conc: 1.68 ug/ml

Instrument :
FID_G
ClientSampleId :
TR-05-032819

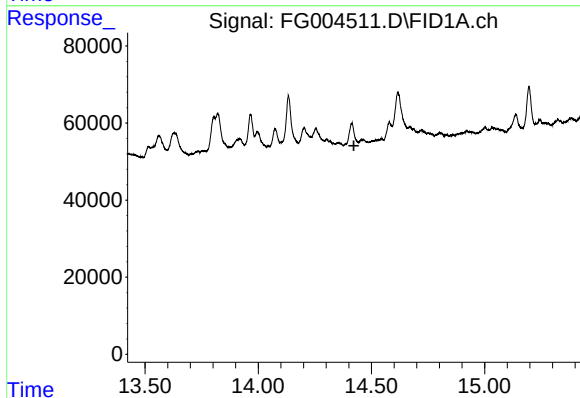


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

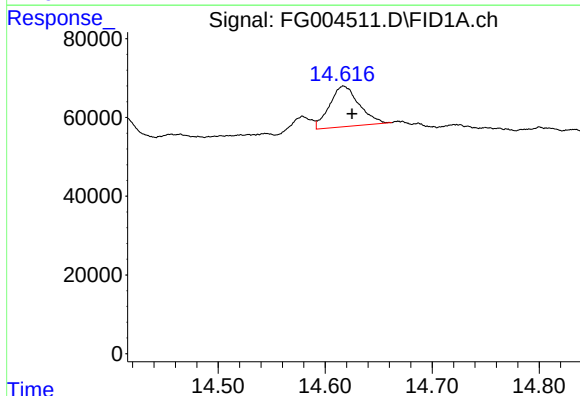


#10 N-TETRACOSANE

R.T.: 14.617 min
Delta R.T.: -0.008 min
Response: 197980
Conc: 1.71 ug/ml

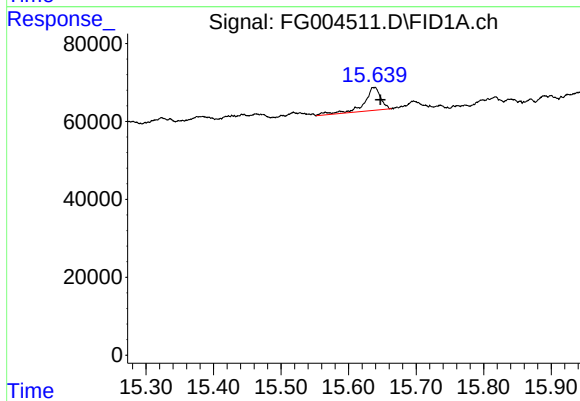

#11 N-HEXACOSANE


R.T.: 15.638 min
Delta R.T.: -0.009 min
Response: 100958
Conc: 0.88 ug/ml

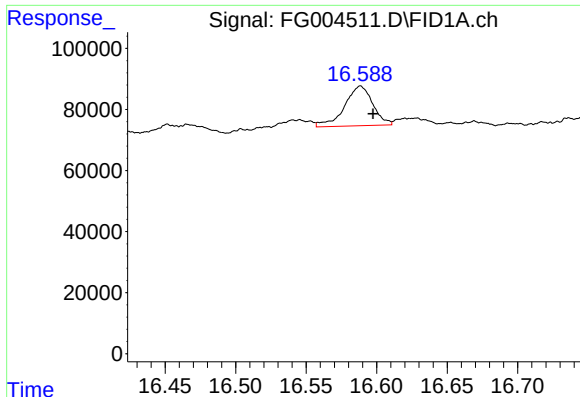

#12 N-OCTACOSANE


R.T.: 16.589 min
Delta R.T.: -0.009 min
Response: 179978
Conc: 1.56 ug/ml

Instrument :
FID_G
ClientSampleId :
TR-05-032819

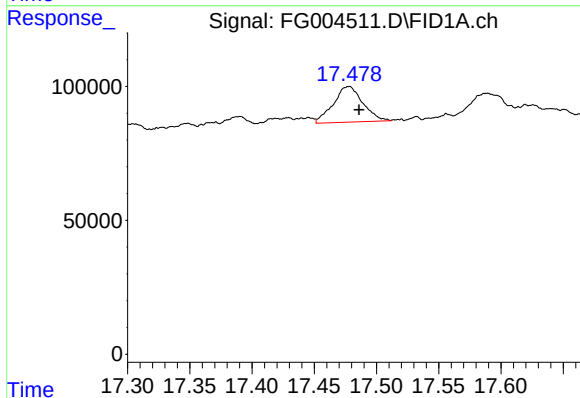


#13 N-TRIACONTANE

R.T.: 17.478 min
Delta R.T.: -0.008 min
Response: 220067
Conc: 1.86 ug/ml

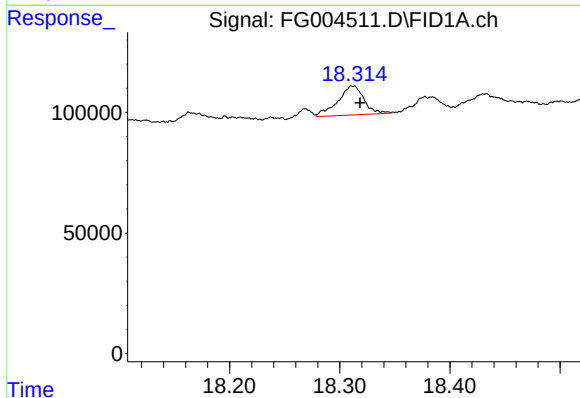


#14 N-DOTRIACONTANE

R.T.: 18.312 min
Delta R.T.: -0.007 min
Response: 198030
Conc: 1.69 ug/ml

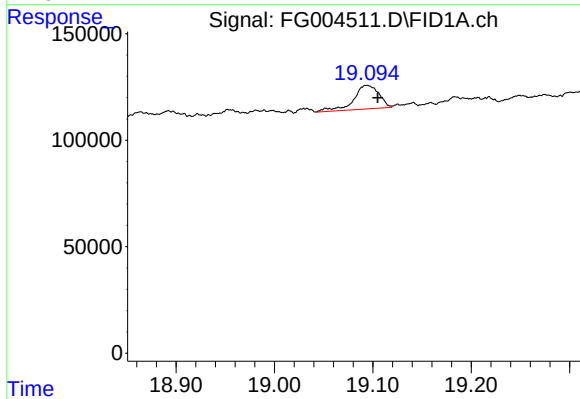

#15 N-TETRATRIACONTANE

R.T.: 19.094 min
Delta R.T.: -0.011 min
Response: 198052
Conc: 1.78 ug/ml

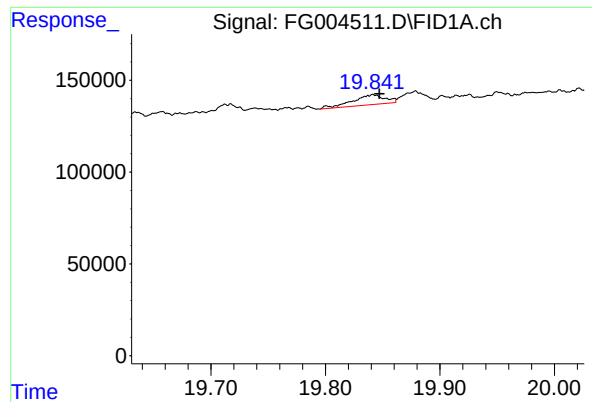

#16 N-HEXATRIACONTANE

R.T.: 19.842 min
Delta R.T.: -0.005 min
Response: 106281
Conc: 0.95 ug/ml

Instrument :
FID_G
ClientSampleId :
TR-05-032819