

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
 Data File : FG004487.D
 Signal(s) : FID1A.ch
 Acq On : 01 Apr 2019 14:30
 Operator : AJ\SJ
 Sample : PB118449BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB118449BS

Integration File: autoint1.e
 Quant Time: Apr 02 00:43:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.411	1674577	16.235 ug/ml
Target Compounds			
2) N-DECANE	4.148	1593574	15.097 ug/ml
3) N-DODECANE	6.170	1615756	15.336 ug/ml
4) N-TETRADECANE	7.962	1650976	15.238 ug/ml
5) N-HEXADECANE	9.562	1709812	15.282 ug/ml
6) N-OCTADECANE	11.003	1726099	15.218 ug/ml
7) N-EICOSANE	12.312	1727494	15.112 ug/ml
8) N-DOCOSANE	13.510	1716432	15.015 ug/ml
10) N-TETRACOSANE	14.614	1755574	15.198 ug/ml
11) N-HEXACOSANE	15.637	1697652	14.809 ug/ml
12) N-OCTACOSANE	16.585	1688103	14.592 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040119\
Data File : FG004487.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2019 14:30
Operator : AJ\SJ
Sample : PB118449BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB118449BS

Integration File: autoint1.e
Quant Time: Apr 02 00:43:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

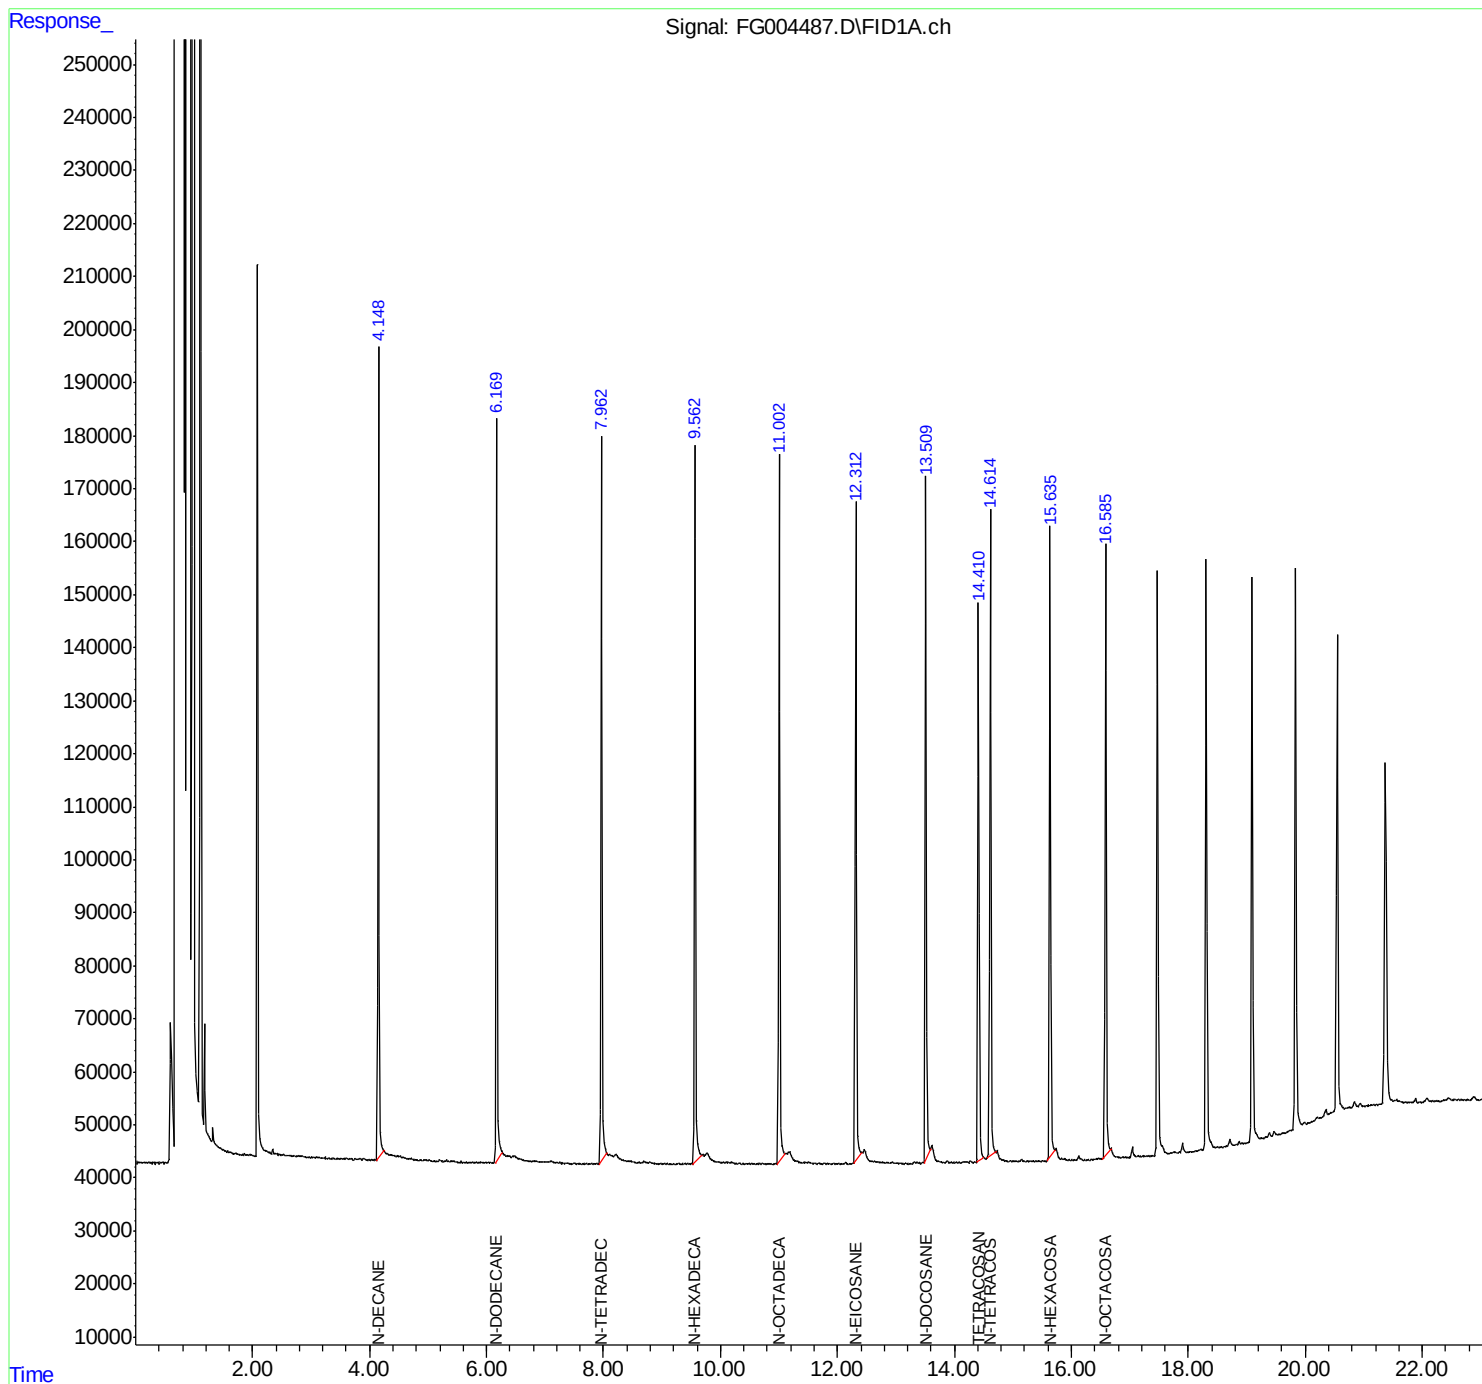


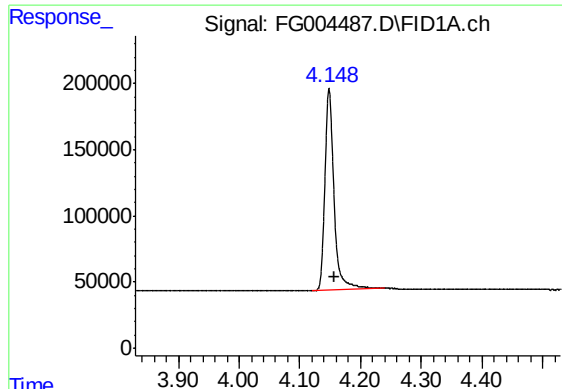

#2 N-DECANE


R.T.: 4.148 min
Delta R.T.: -0.008 min
Response: 1593574
Conc: 15.10 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118449BS

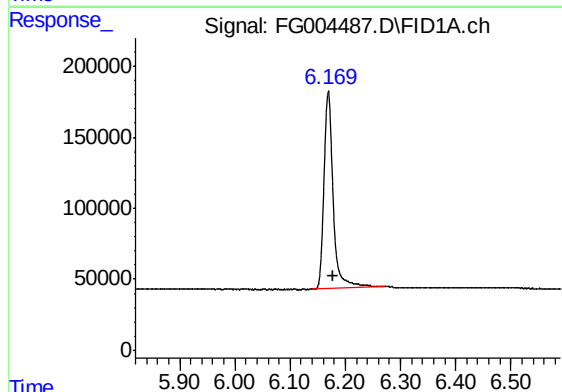


#3 N-DODECANE

R.T.: 6.170 min
Delta R.T.: -0.009 min
Response: 1615756
Conc: 15.34 ug/ml

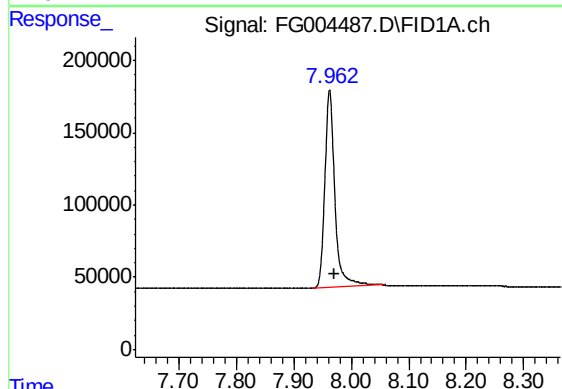


#4 N-TETRADECANE

R.T.: 7.962 min
Delta R.T.: -0.009 min
Response: 1650976
Conc: 15.24 ug/ml

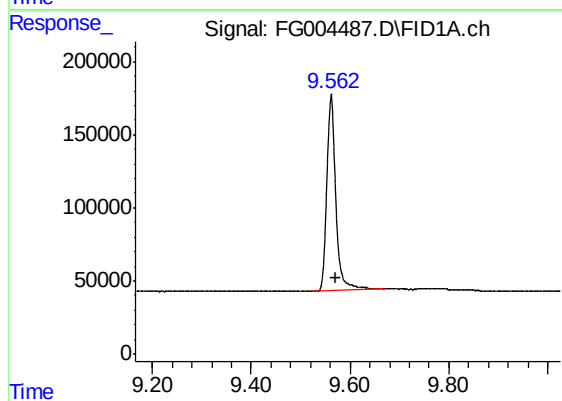

#5 N-HEXADECANE


R.T.: 9.562 min
Delta R.T.: -0.010 min
Response: 1709812
Conc: 15.28 ug/ml

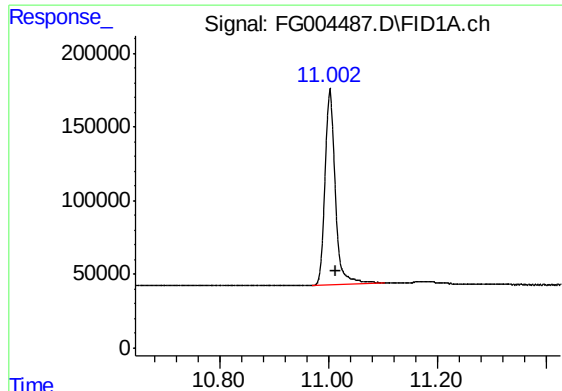

#6 N-OCTADECANE


R.T.: 11.003 min
Delta R.T.: -0.010 min
Response: 1726099
Conc: 15.22 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118449BS

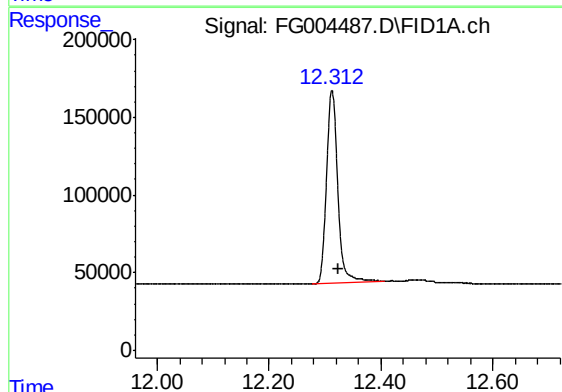


#7 N-EICOSANE

R.T.: 12.312 min
Delta R.T.: -0.011 min
Response: 1727494
Conc: 15.11 ug/ml

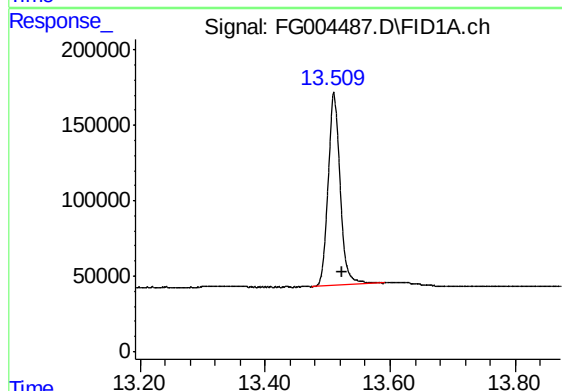


#8 N-DOCOSANE

R.T.: 13.510 min
Delta R.T.: -0.013 min
Response: 1716432
Conc: 15.02 ug/ml

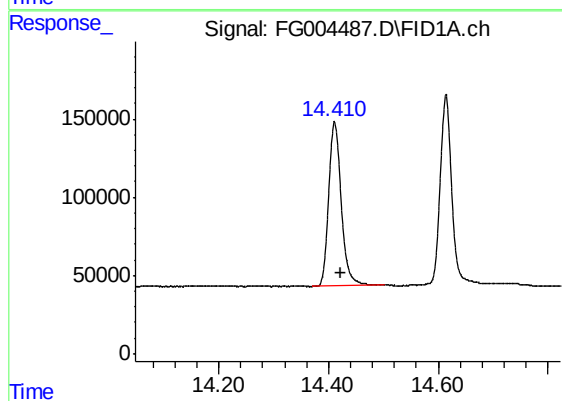

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.411 min
Delta R.T.: -0.012 min
Response: 1674577
Conc: 16.23 ug/ml

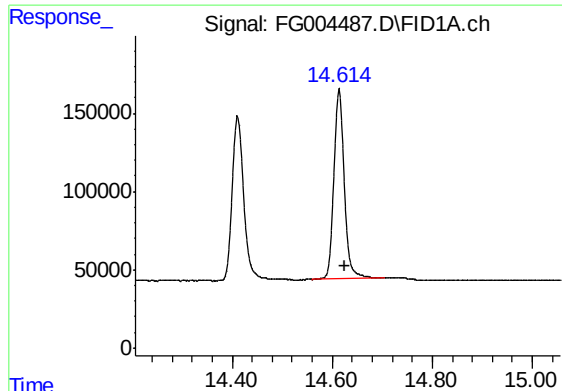

#10 N-TETRACOSANE


R.T.: 14.614 min
Delta R.T.: -0.011 min
Response: 1755574
Conc: 15.20 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118449BS

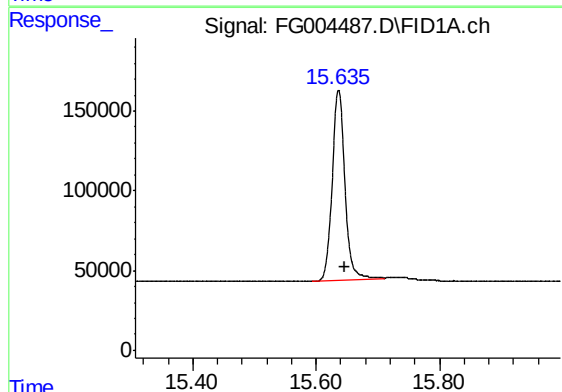

#11 N-HEXACOSANE

R.T.: 15.637 min
Delta R.T.: -0.010 min
Response: 1697652
Conc: 14.81 ug/ml

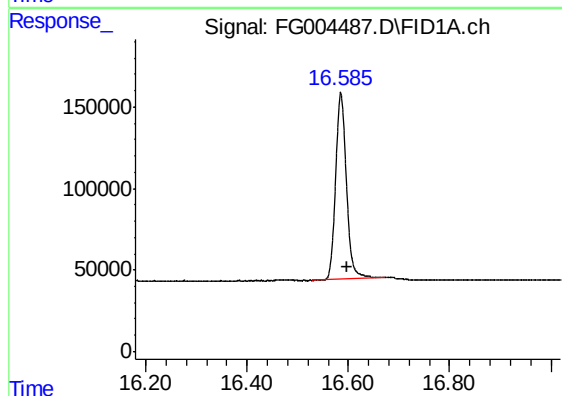

#12 N-OCTACOSANE

R.T.: 16.585 min
Delta R.T.: -0.012 min
Response: 1688103
Conc: 14.59 ug/ml