

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040122\
Data File : FG009490.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2022 10:02
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 13:56:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 01 13:54:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	2422120	17.980 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040122\
Data File : FG009490.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2022 10:02
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 13:56:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG040122.M
Quant Title :
QLast Update : Fri Apr 01 13:54:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

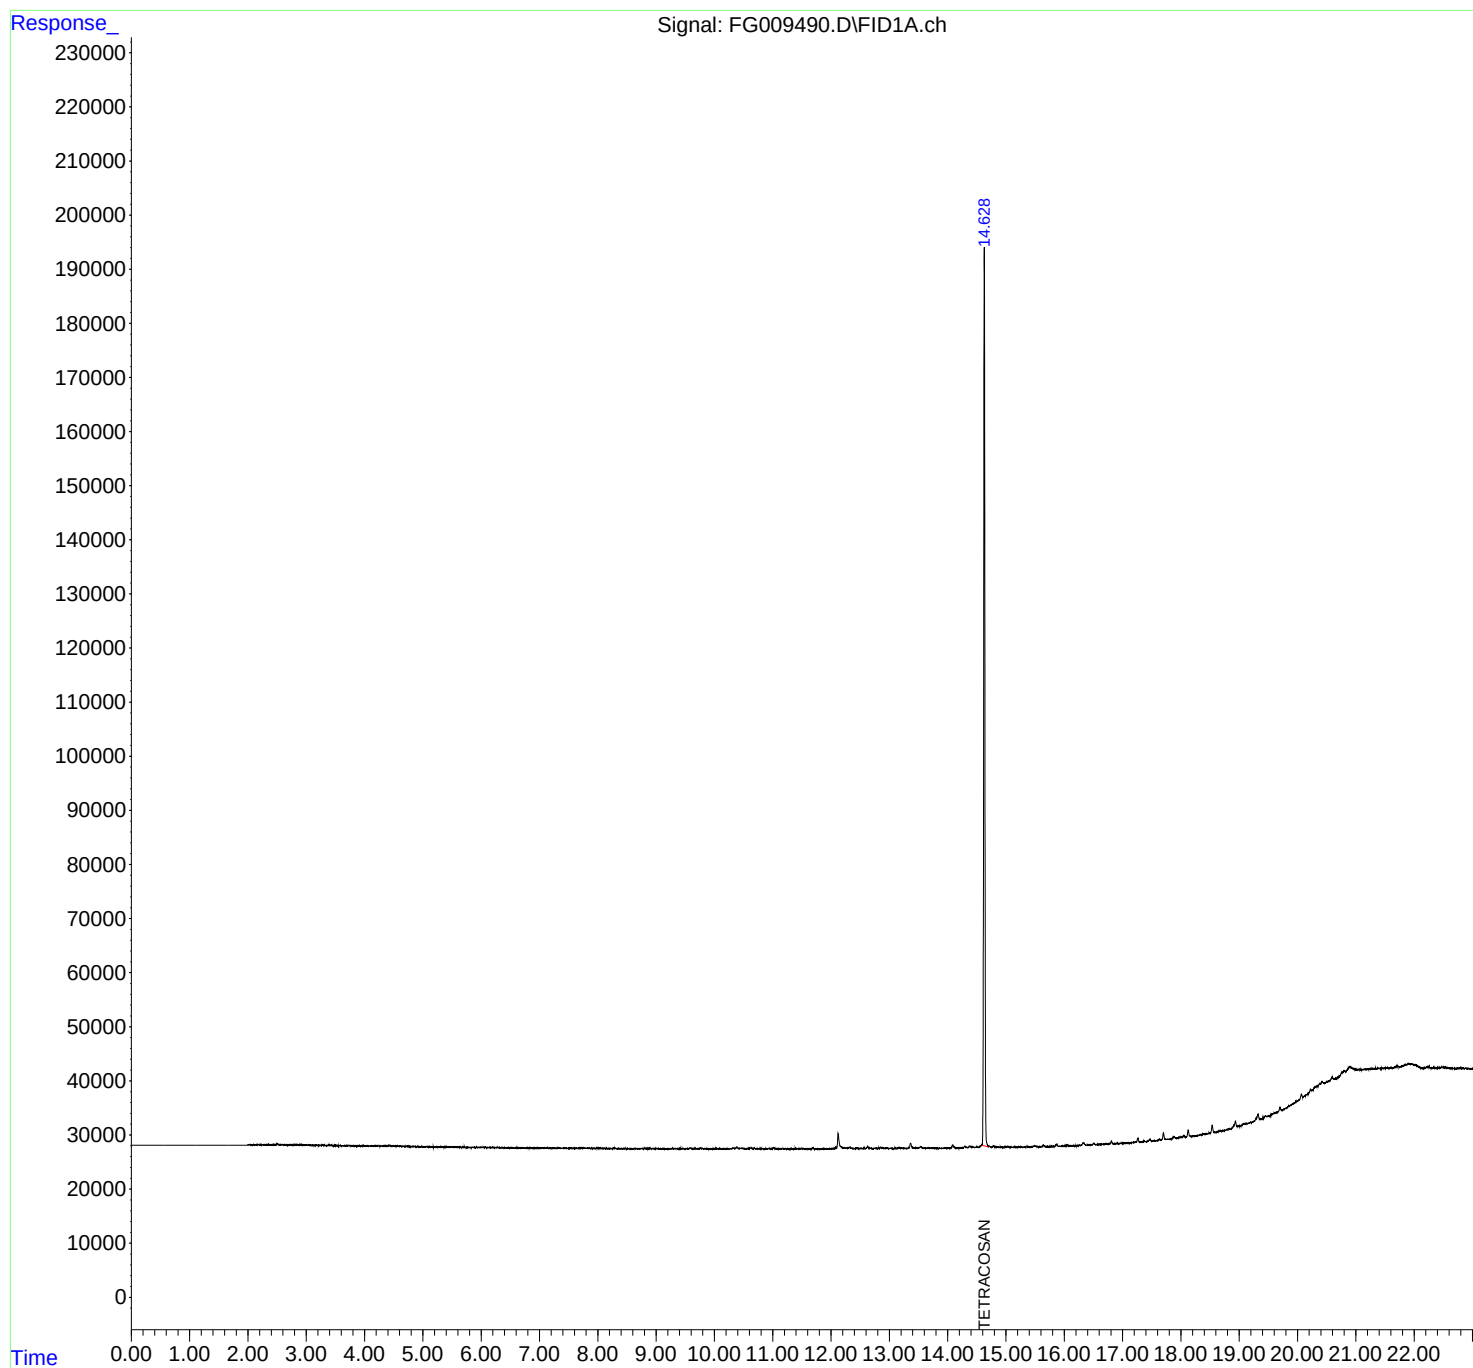

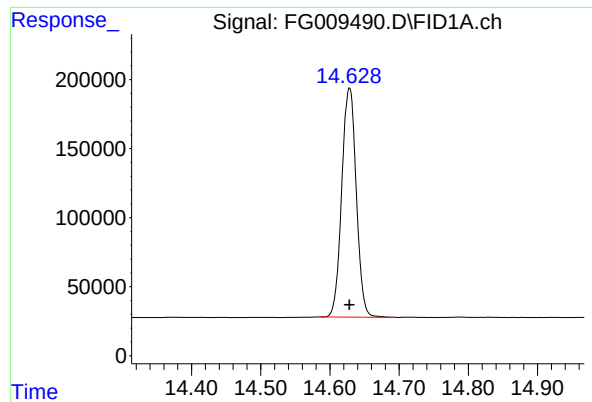

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.628 min
Delta R.T.: 0.000 min
Response: 2422120
Conc: 17.98 ug/ml

Instrument :

FID_G

ClientSampleId :