

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040125AR\
Data File : FG015592.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2025 08:12
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Apr 02 01:14:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 031725.M
Quant Title : GC Extractables
QLast Update : Tue Mar 18 05:13:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	Benzo[a]anthracene (C...	15.187	1085185	8.001 ug/ml
15) T	Chrysene (C27.41)	15.187	1085185	7.752 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040125AR\
Data File : FG015592.D
Signal(s) : FID1A.ch
Acq On : 01 Apr 2025 08:12
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Apr 02 01:14:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 031725.M
Quant Title : GC Extractables
QLast Update : Tue Mar 18 05:13:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

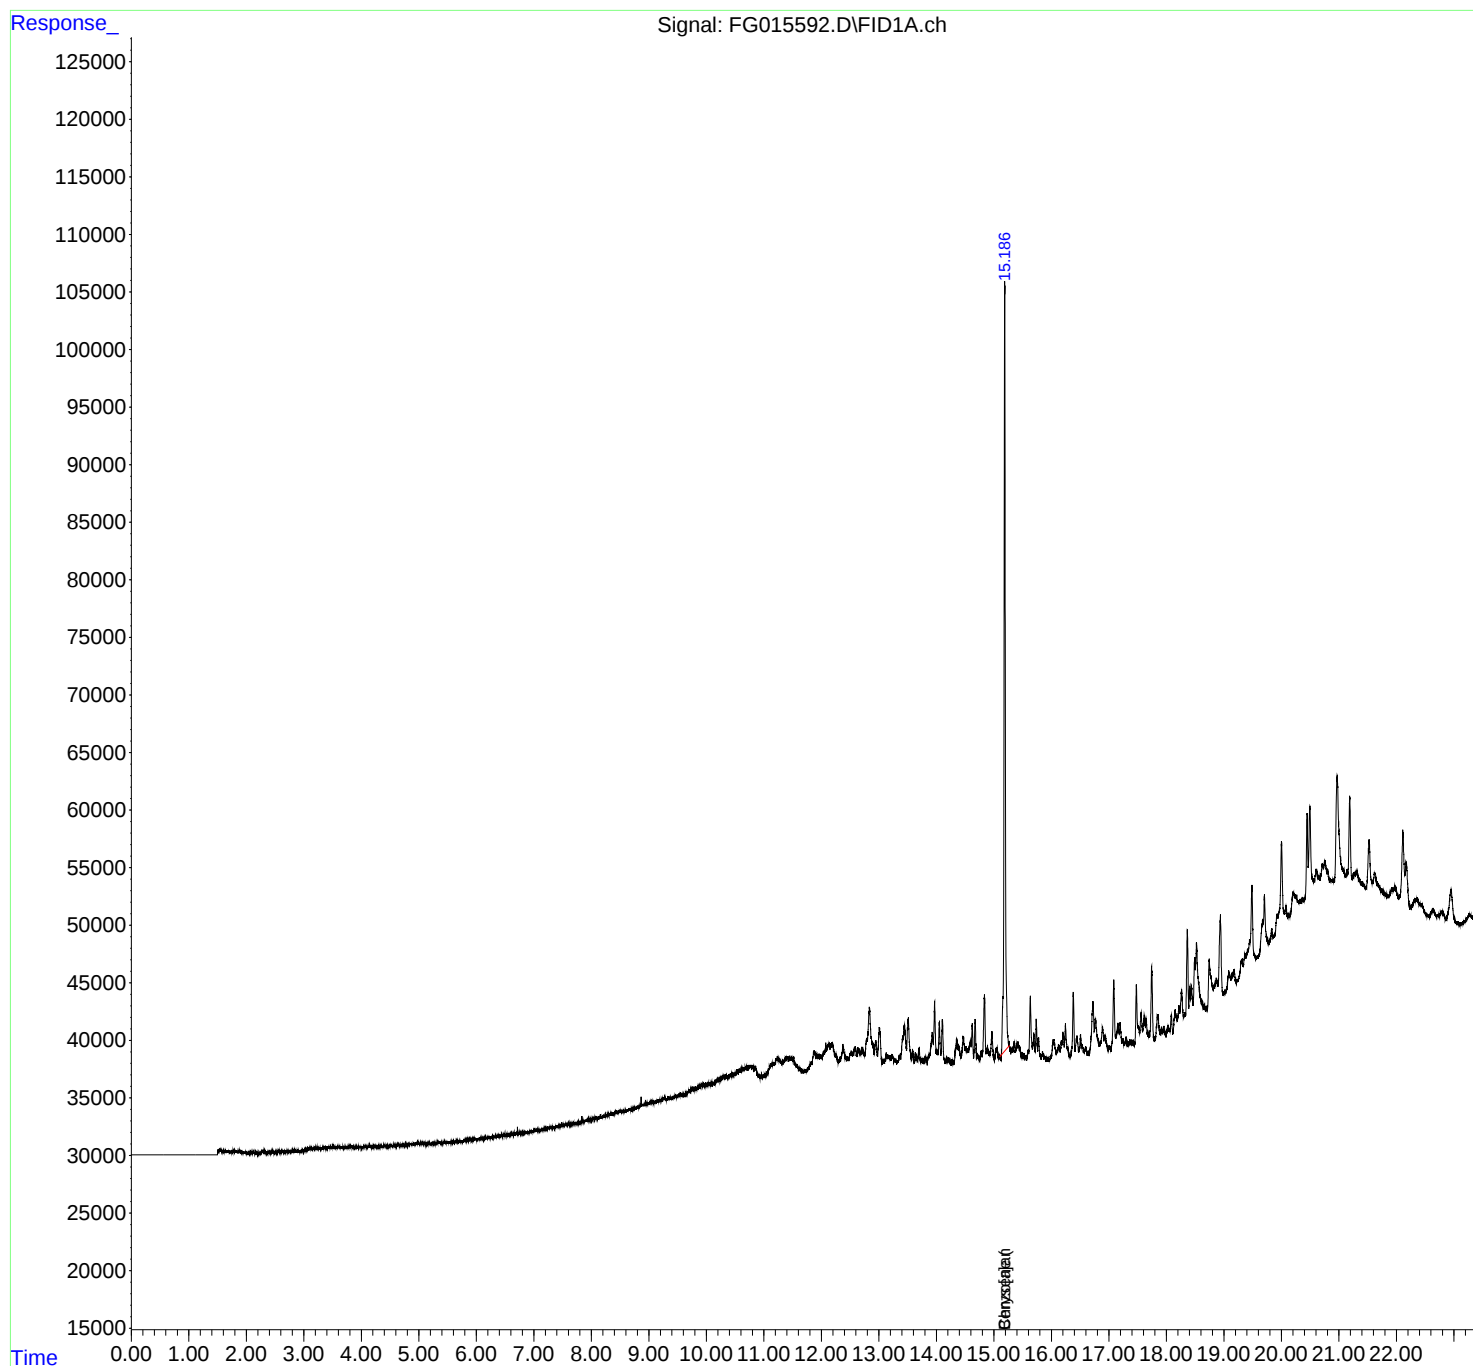


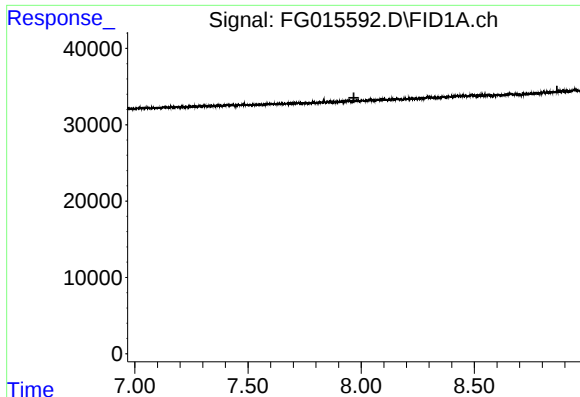

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.968 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
MECL2

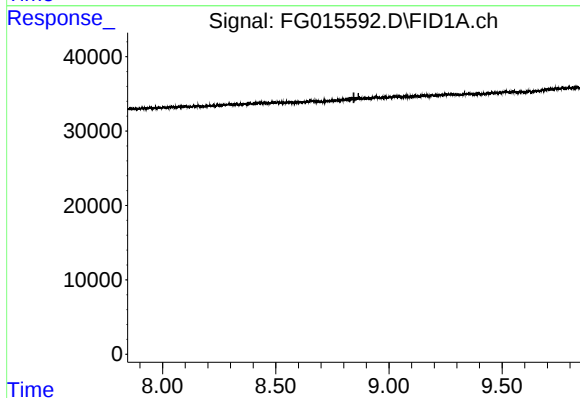


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

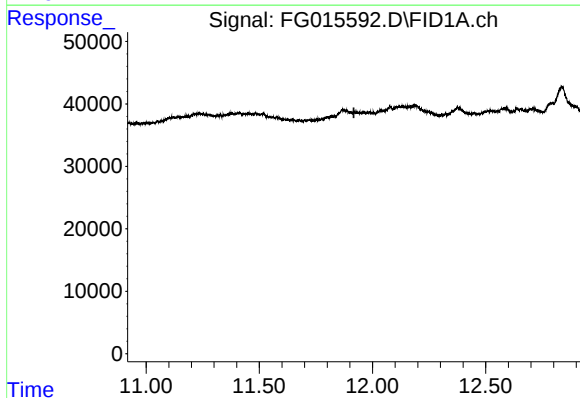


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.918 min
Response: 0
Conc: N.D.

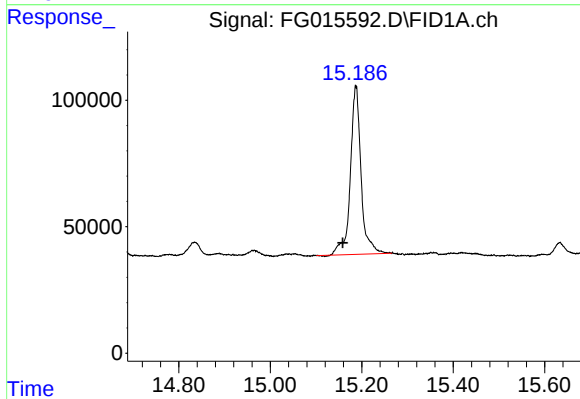

#14 Benzo[a]anthracene (C26.37)

R.T.: 15.187 min
Delta R.T.: 0.028 min
Response: 1085185
Conc: 8.00 ug/ml

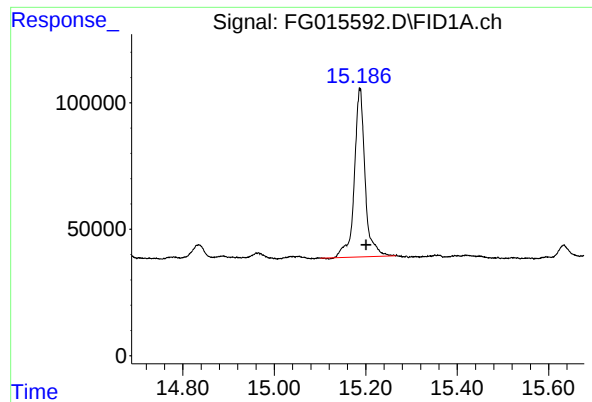

#15 Chrysene (C27.41)

R.T.: 15.187 min
Delta R.T.: -0.014 min
Response: 1085185
Conc: 7.75 ug/ml

Instrument :
FID_G
ClientSampleId :
MECL2