

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004517.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 10:01
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 02 14:03:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.169	2191913	20.804 ug/ml
12) N-OCTACOSANE	16.587	2402532	20.767 ug/ml
13) N-TRIACONTANE	17.473	117005	0.986 ug/ml
14) N-DOTRIACONTANE	18.308	150101	1.280 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004517.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 10:01
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 02 14:03:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

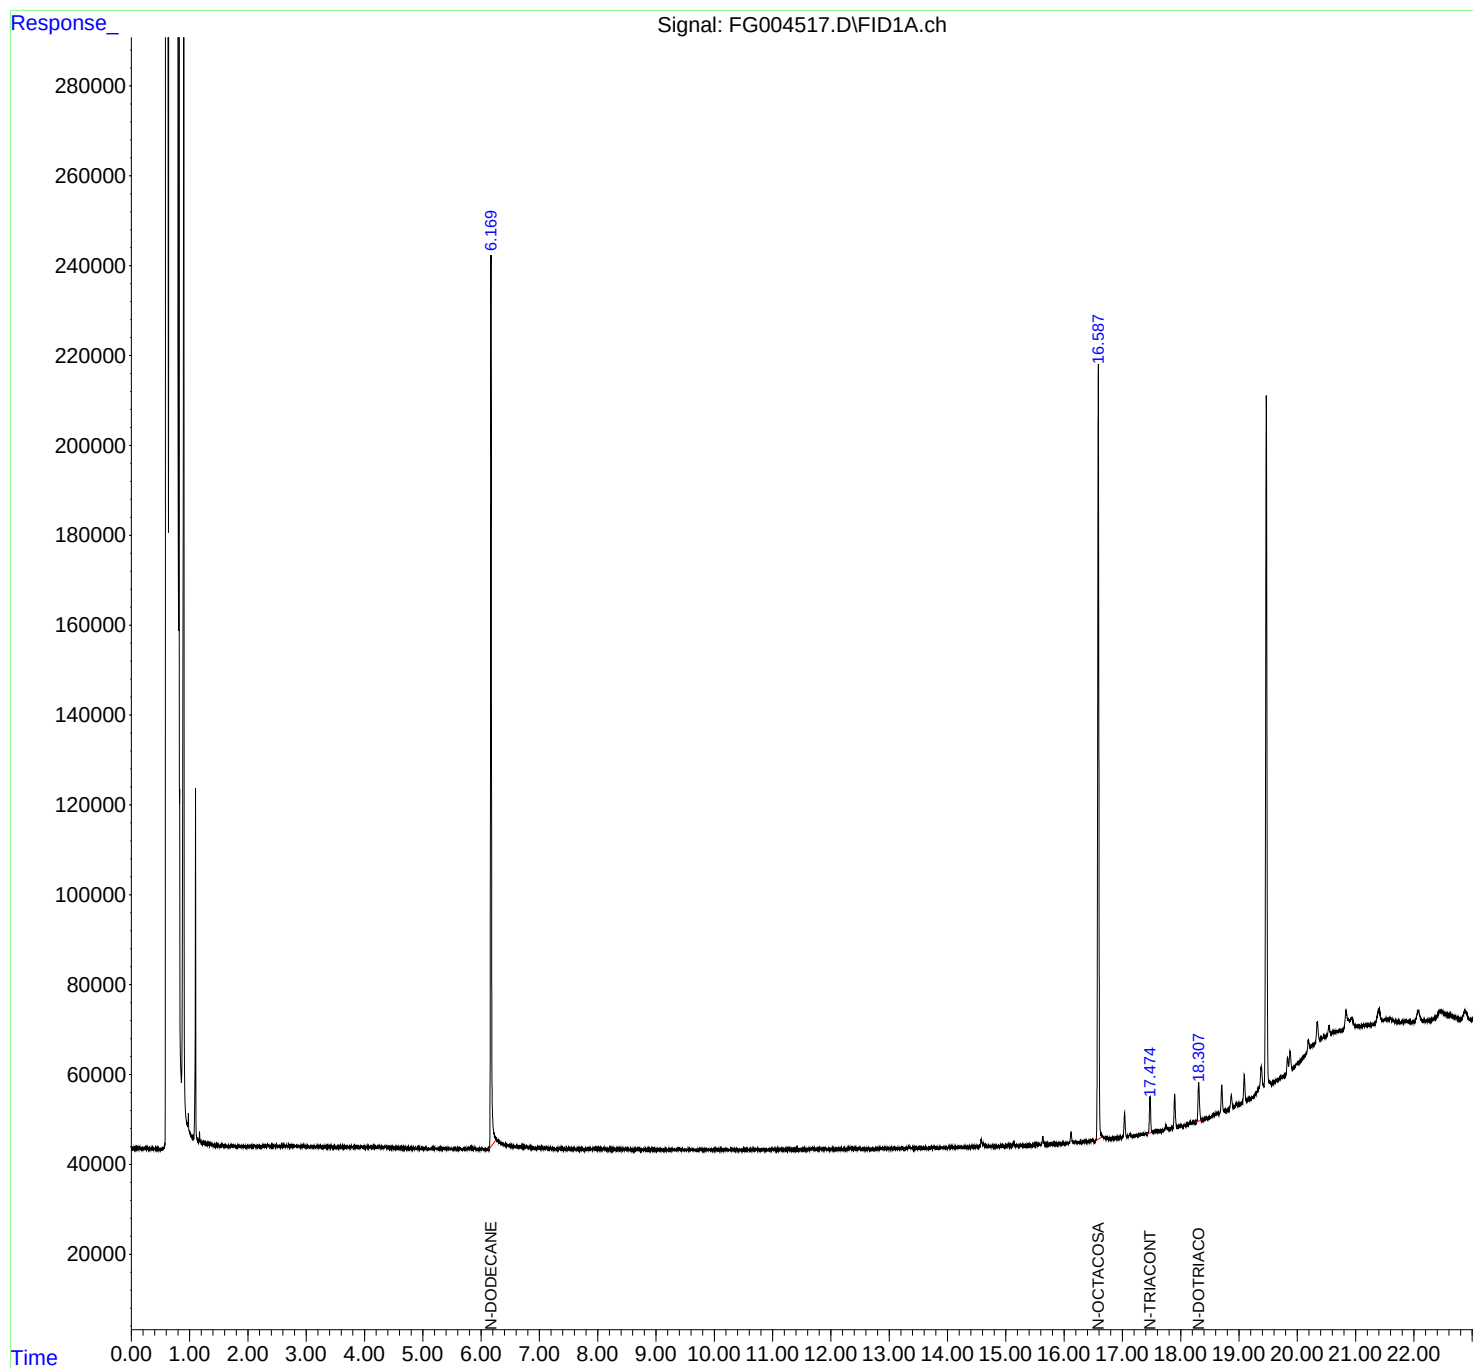


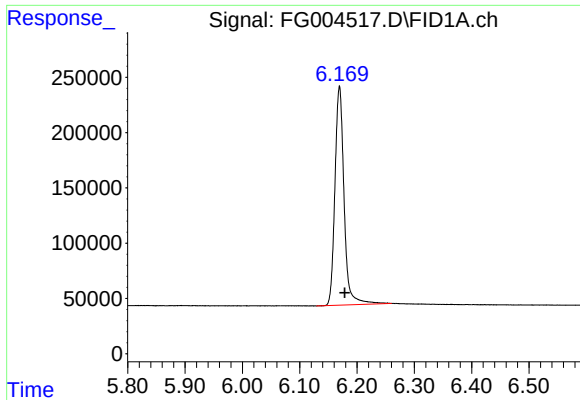

#3 N-DODECANE


R.T.: 6.169 min
Delta R.T.: -0.009 min
Response: 2191913
Conc: 20.80 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

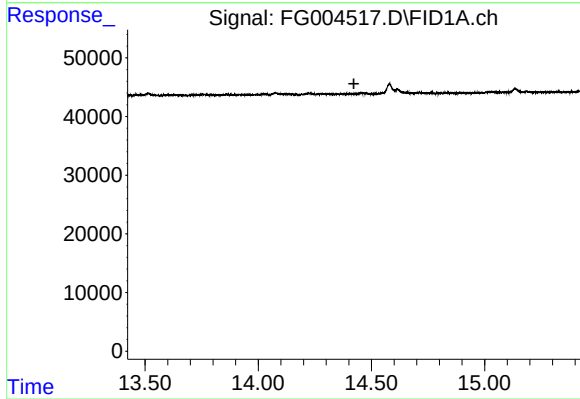


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

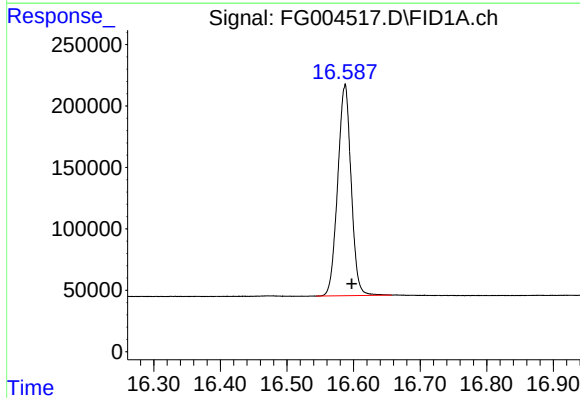


#12 N-OCTACOSANE

R.T.: 16.587 min
Delta R.T.: -0.010 min
Response: 2402532
Conc: 20.77 ug/ml

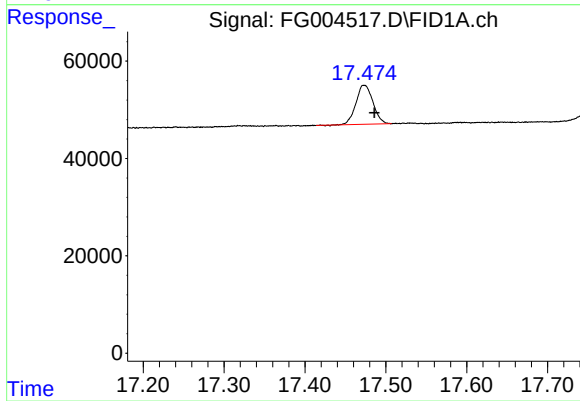

#13 N-TRIACONTANE

R.T.: 17.473 min
Delta R.T.: -0.013 min
Response: 117005
Conc: 0.99 ug/ml

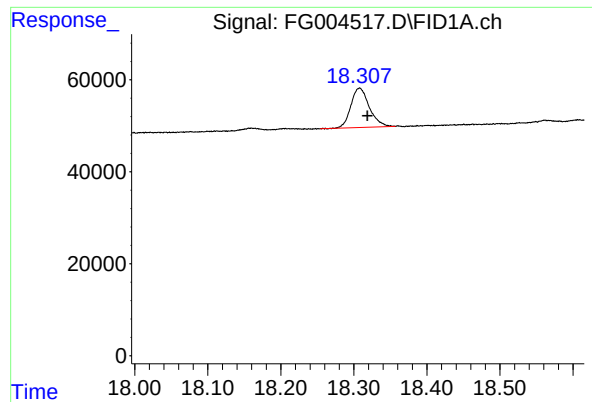

#14 N-DOTRIACONTANE

R.T.: 18.308 min
Delta R.T.: -0.011 min
Response: 150101
Conc: 1.28 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER