

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
 Data File : FG004520.D
 Signal(s) : FID1A.ch
 Acq On : 02 Apr 2019 11:34
 Operator : AJ\SJ
 Sample : K2056-01 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 CS-7

Integration File: autoint1.e
 Quant Time: Apr 02 14:03:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.411	389709	3.778 ug/ml
Target Compounds			
7) N-EICOSANE	12.363	2353924	20.591 ug/ml
8) N-DOCOSANE	13.532	298129	2.608 ug/ml
10) N-TETRACOSANE	14.590	2451412	21.221 ug/ml
11) N-HEXACOSANE	15.663	166016	1.448 ug/ml
12) N-OCTACOSANE	16.610	581677	5.028 ug/ml
13) N-TRIACONTANE	17.477	217932	1.837 ug/ml
14) N-DOTRIACONTANE	18.301	286983	2.447 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004520.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 11:34
Operator : AJ\SJ
Sample : K2056-01 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CS-7

Integration File: autoint1.e
Quant Time: Apr 02 14:03:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

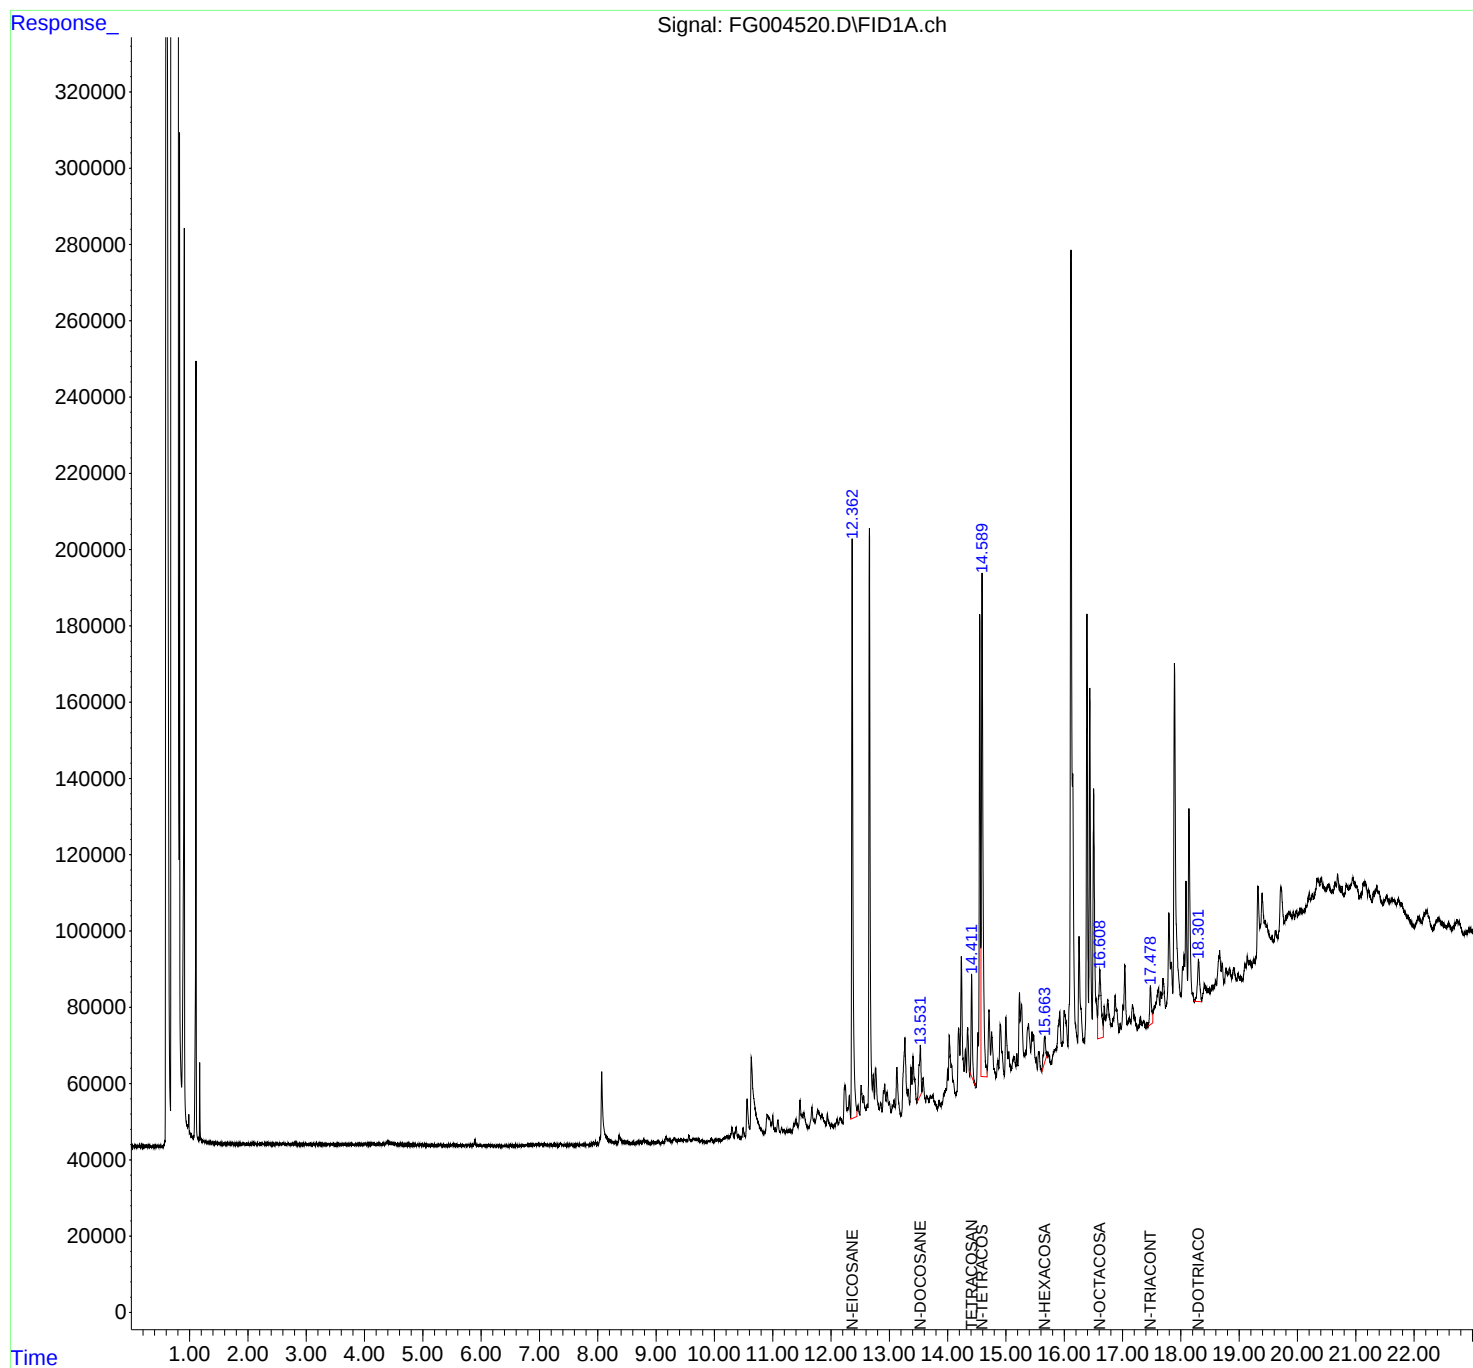


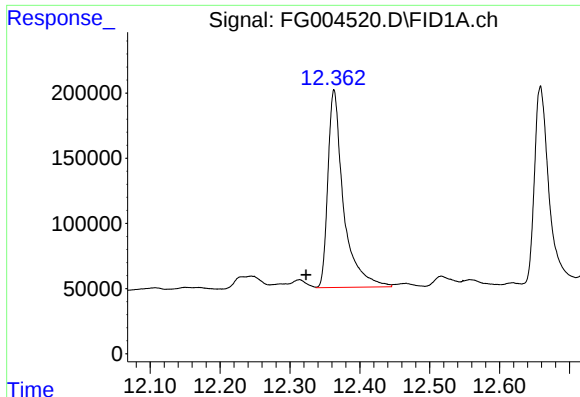

#7 N-EICOSANE


R.T.: 12.363 min
Delta R.T.: 0.040 min
Response: 2353924
Conc: 20.59 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-7

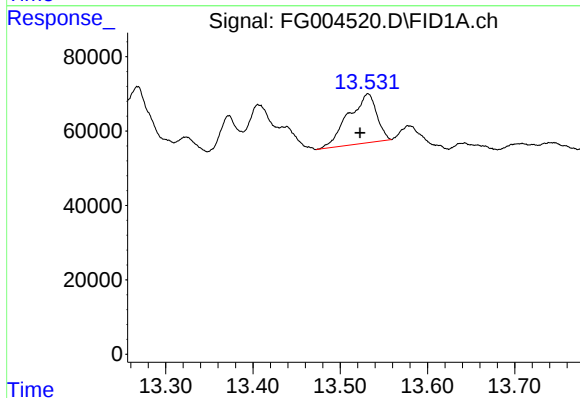


#8 N-DOCOSANE

R.T.: 13.532 min
Delta R.T.: 0.009 min
Response: 298129
Conc: 2.61 ug/ml

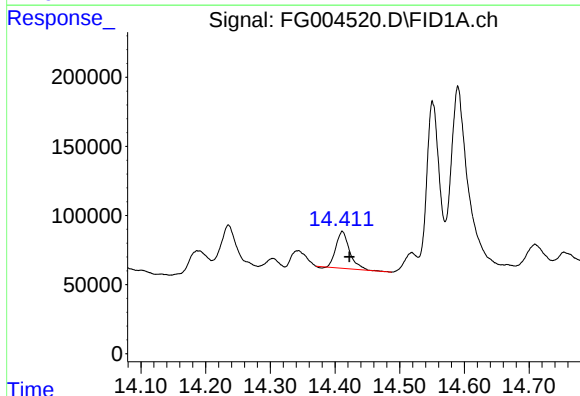


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.411 min
Delta R.T.: -0.011 min
Response: 389709
Conc: 3.78 ug/ml

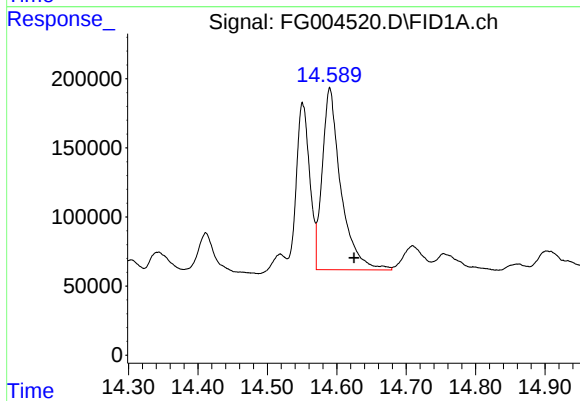

#10 N-TETRACOSANE


R.T.: 14.590 min
Delta R.T.: -0.035 min
Response: 2451412
Conc: 21.22 ug/ml

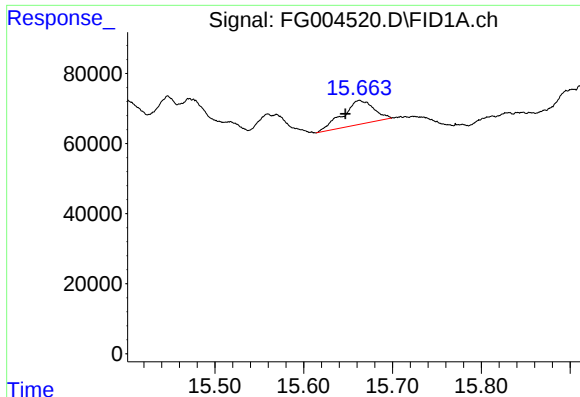

#11 N-HEXACOSANE


R.T.: 15.663 min
Delta R.T.: 0.016 min
Response: 166016
Conc: 1.45 ug/ml

Instrument :
FID_G
ClientSampleId :
CS-7

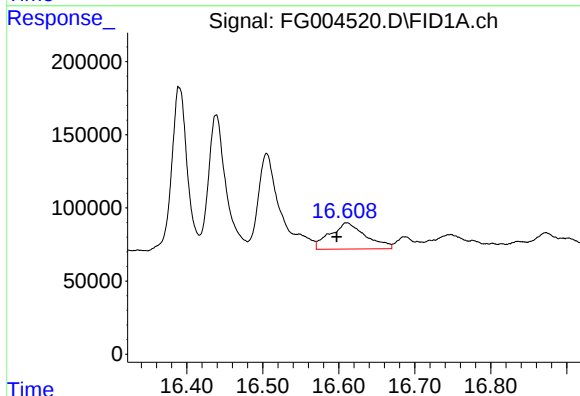


#12 N-OCTACOSANE

R.T.: 16.610 min
Delta R.T.: 0.013 min
Response: 581677
Conc: 5.03 ug/ml

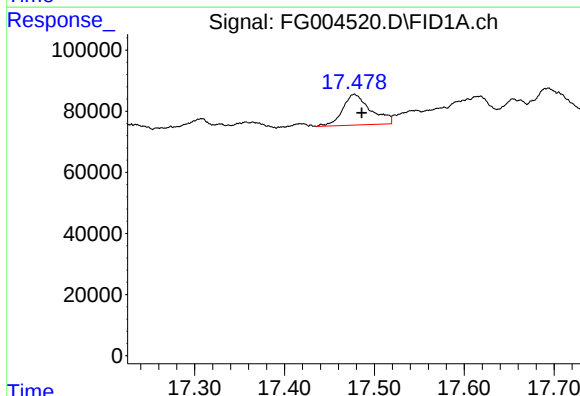

#13 N-TRIACONTANE

R.T.: 17.477 min
Delta R.T.: -0.008 min
Response: 217932
Conc: 1.84 ug/ml

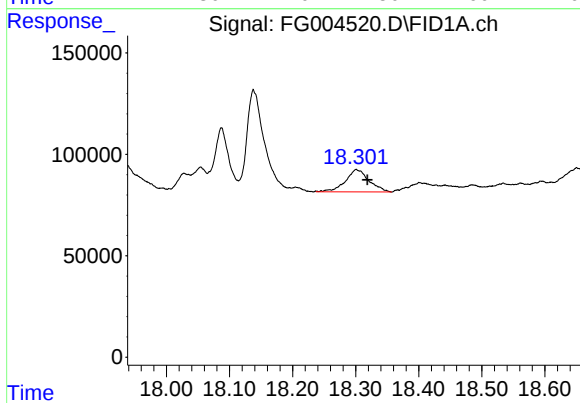

#14 N-DOTRIACONTANE

R.T.: 18.301 min
Delta R.T.: -0.018 min
Response: 286983
Conc: 2.45 ug/ml