

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004527.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 15:26
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 02 23:31:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.169	2299223	21.823 ug/ml
12)	N-OCTACOSANE	16.588	2488540	21.511 ug/ml
13)	N-TRIACONTANE	17.474	157435	1.327 ug/ml
14)	N-DOTRIACONTANE	18.307	223360	1.905 ug/ml
15)	N-TETRATRIACONTANE	19.092	120129	1.078 ug/ml
18)	N-TETRACONTANE	21.404	231892	2.144 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004527.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 15:26
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 02 23:31:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

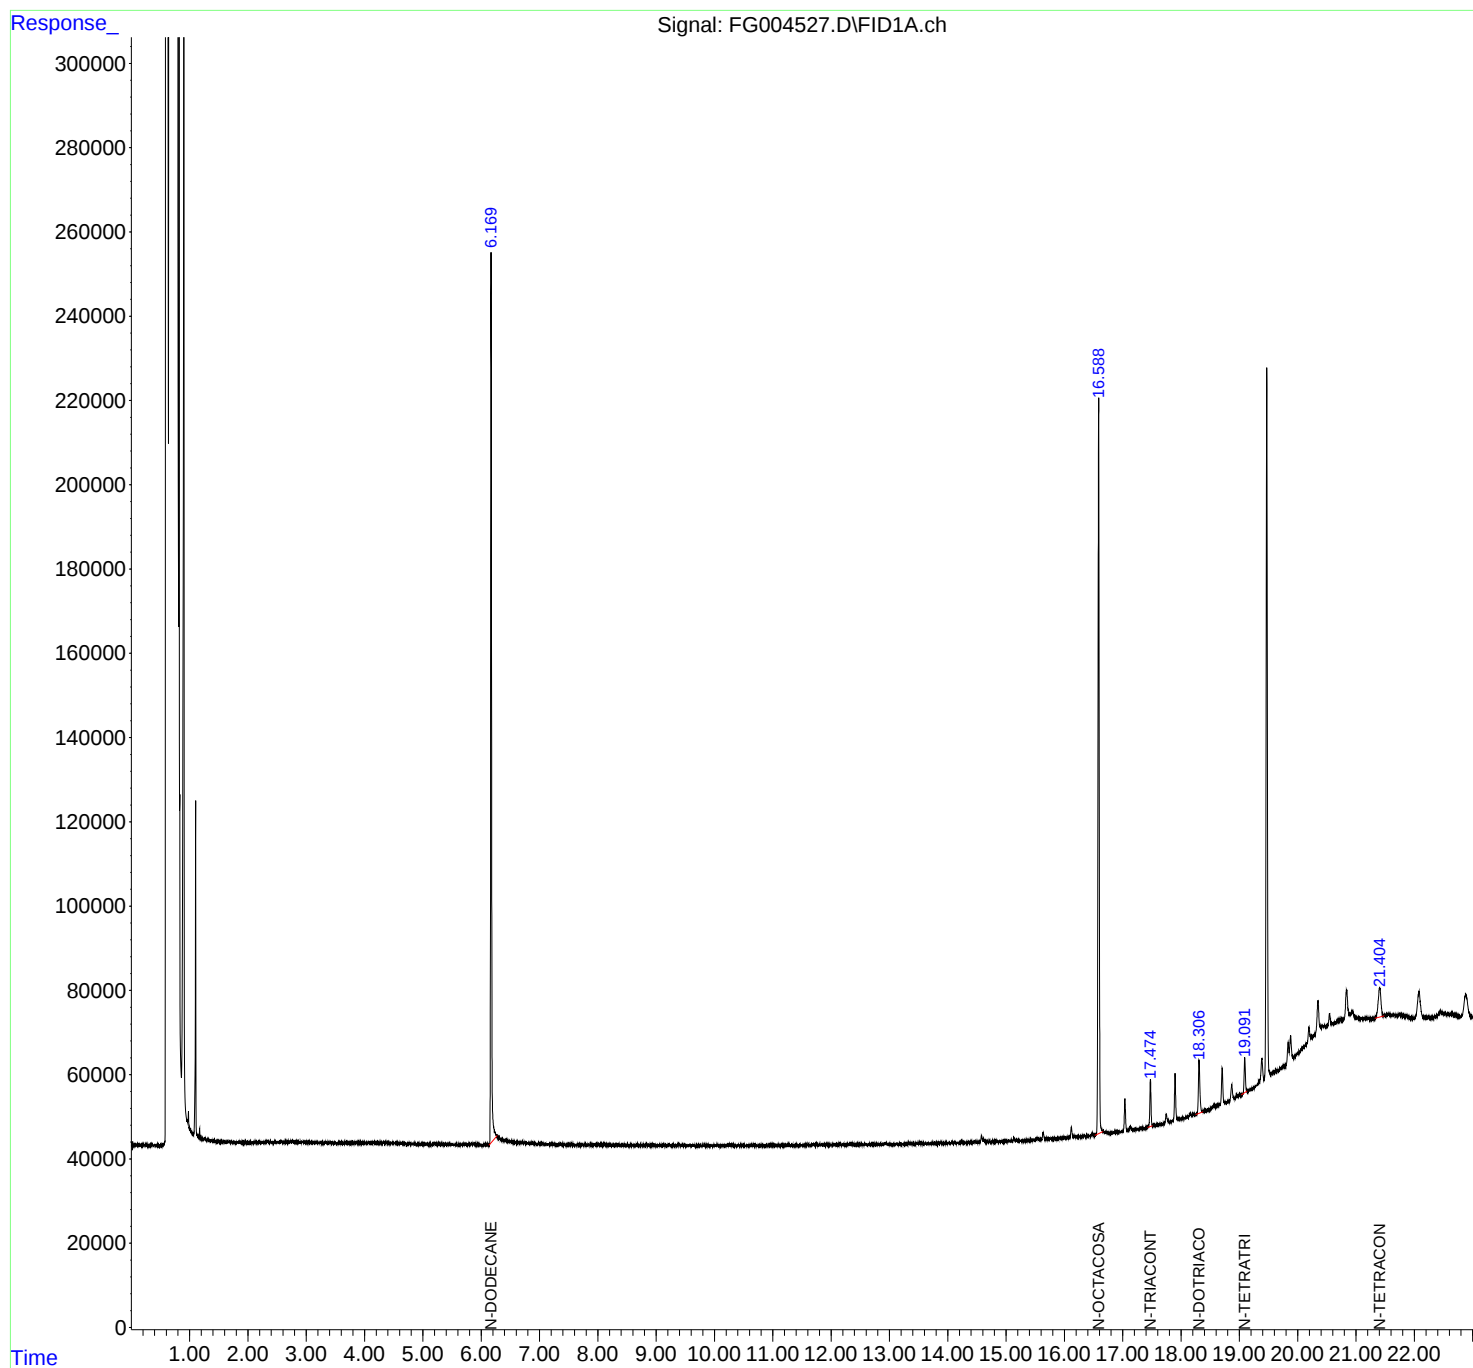


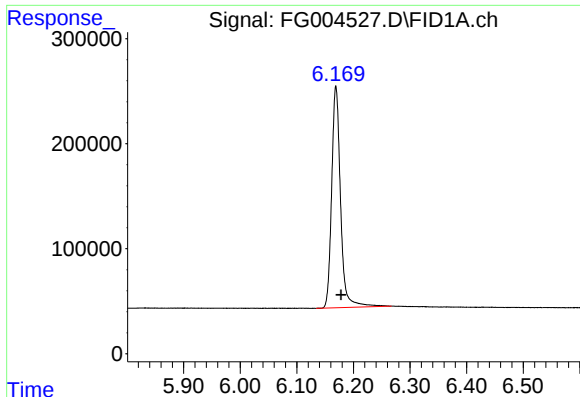

#3 N-DODECANE


R.T.: 6.169 min
Delta R.T.: -0.009 min
Response: 2299223
Conc: 21.82 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

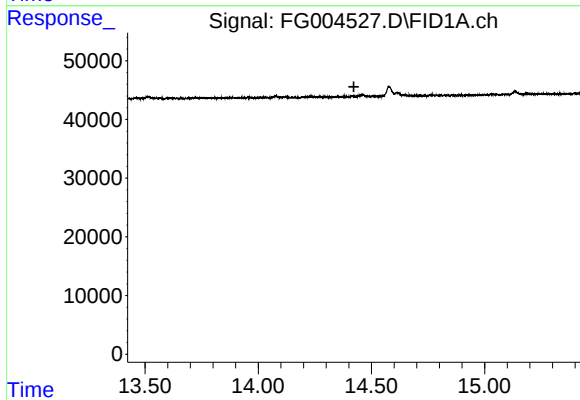


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

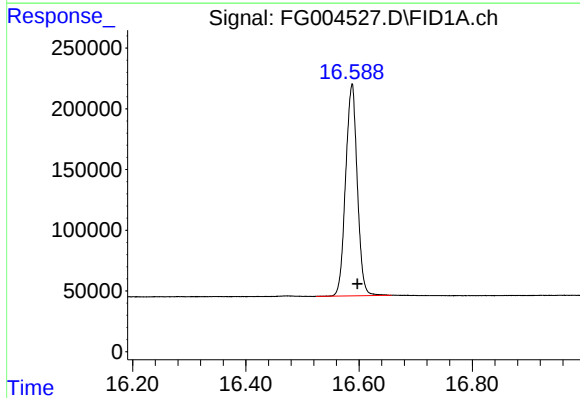


#12 N-OCTACOSANE

R.T.: 16.588 min
Delta R.T.: -0.010 min
Response: 2488540
Conc: 21.51 ug/ml

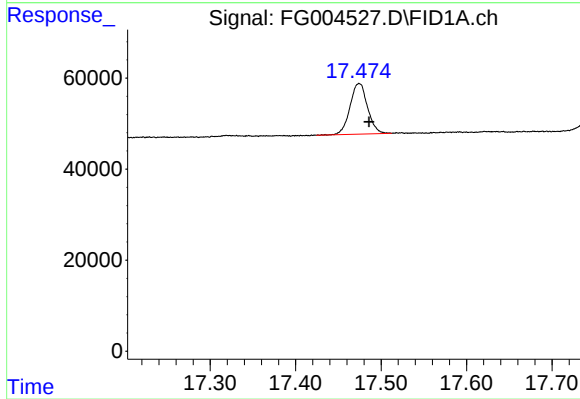

#13 N-TRIACONTANE


R.T.: 17.474 min
Delta R.T.: -0.012 min
Response: 157435
Conc: 1.33 ug/ml

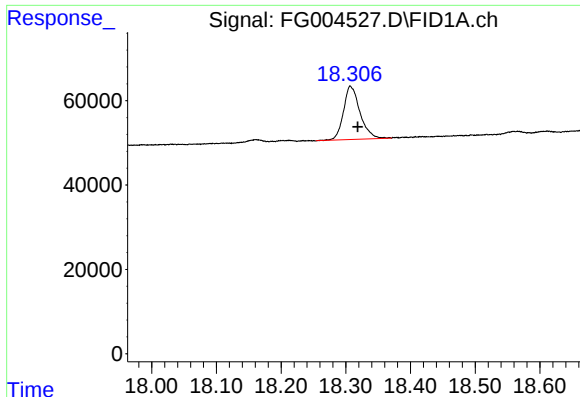

#14 N-DOTRIACONTANE


R.T.: 18.307 min
Delta R.T.: -0.011 min
Response: 223360
Conc: 1.90 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

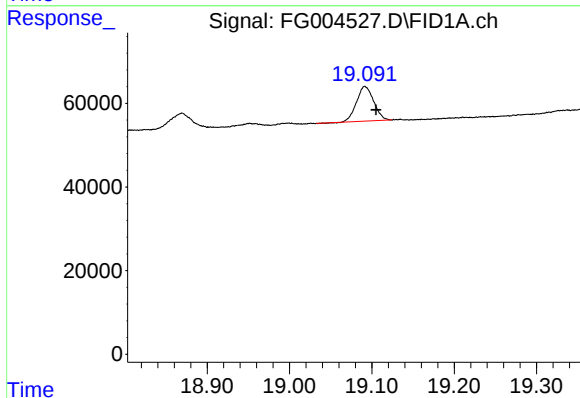

#15 N-TETRATRIACONTANE

R.T.: 19.092 min
Delta R.T.: -0.014 min
Response: 120129
Conc: 1.08 ug/ml

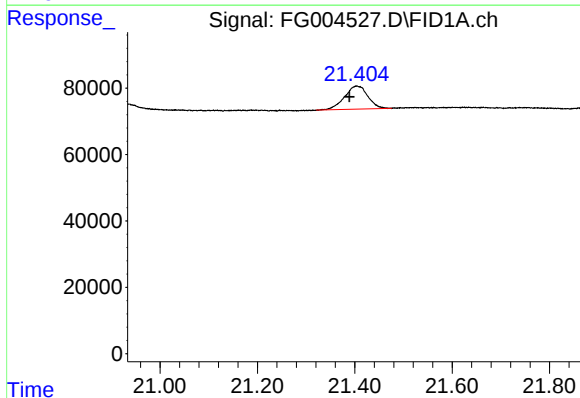

#18 N-TETRACONTANE

R.T.: 21.404 min
Delta R.T.: 0.015 min
Response: 231892
Conc: 2.14 ug/ml