

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004533.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 18:31
Operator : AJ\SJ
Sample : K2182-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S7C(12-20)COMP

Integration File: autoint1.e
Quant Time: Apr 02 23:32:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.411	1323057	12.827 ug/ml
Target Compounds			
4) N-TETRADECANE	8.031f	77050	0.711 ug/ml
7) N-EICOSANE	12.367	840552	7.353 ug/ml
10) N-TETRACOSANE	14.596	955899	8.275 ug/ml
12) N-OCTACOSANE	16.625	225671	1.951 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004533.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 18:31
Operator : AJ\SJ
Sample : K2182-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S7C(12-20)COMP

Integration File: autoint1.e
Quant Time: Apr 02 23:32:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

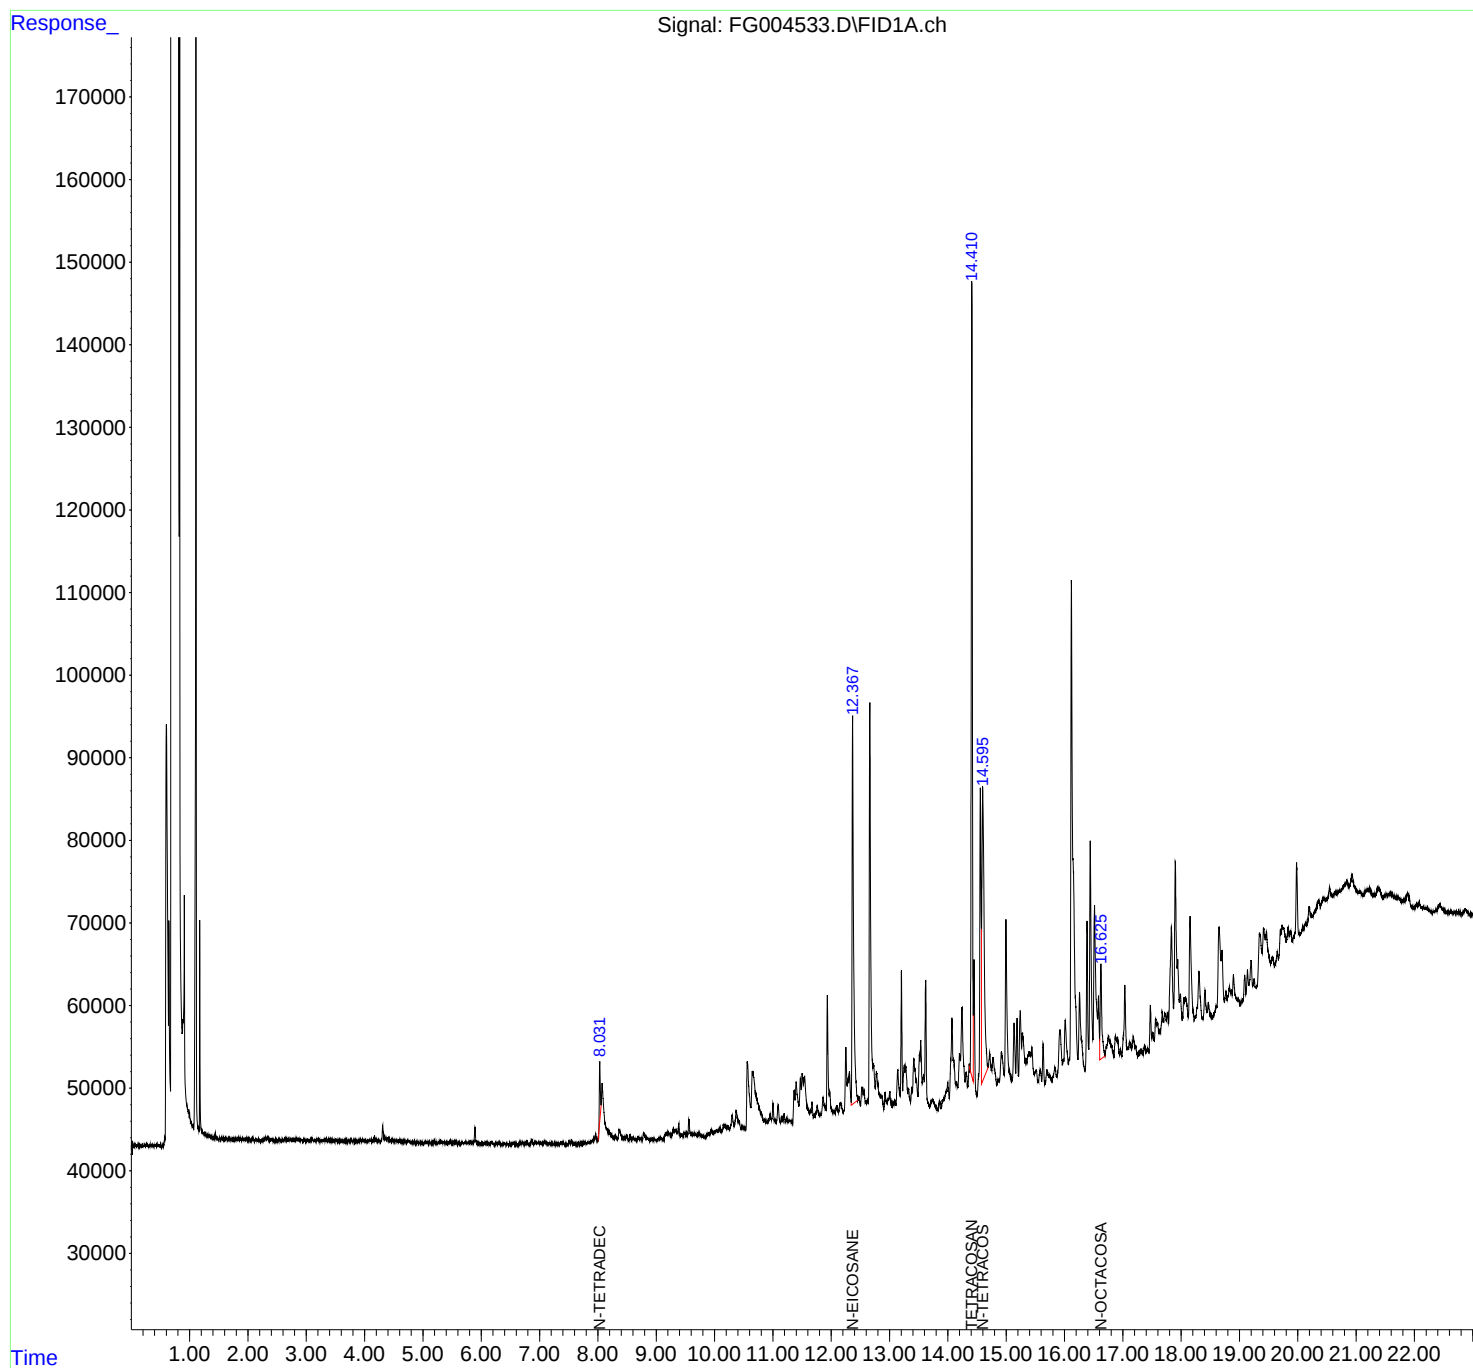


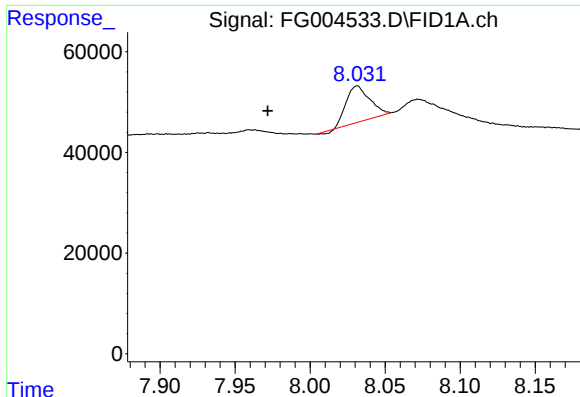

#4 N-TETRADECANE


R.T.: 8.031 min
Delta R.T.: 0.060 min
Response: 77050
Conc: 0.71 ug/ml

Instrument :
FID_G
ClientSampleId :
S7C(12-20)COMP

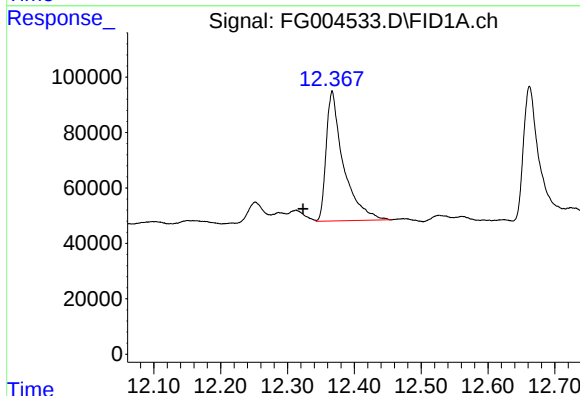


#7 N-EICOSANE

R.T.: 12.367 min
Delta R.T.: 0.044 min
Response: 840552
Conc: 7.35 ug/ml

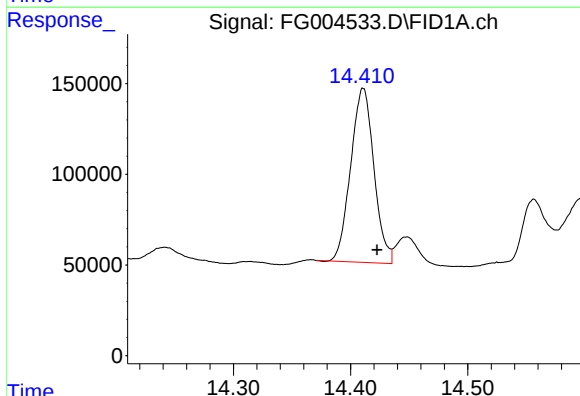


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.411 min
Delta R.T.: -0.012 min
Response: 1323057
Conc: 12.83 ug/ml

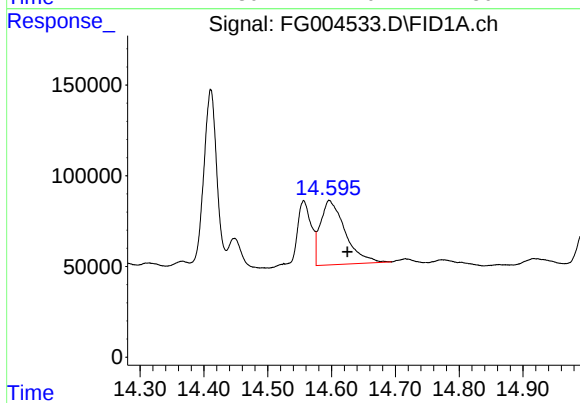

#10 N-TETRACOSANE

R.T.: 14.596 min
Delta R.T.: -0.029 min
Response: 955899
Conc: 8.28 ug/ml

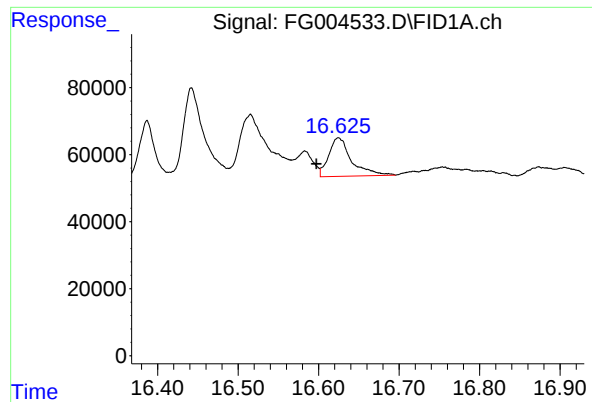

#12 N-OCTACOSANE

R.T.: 16.625 min
Delta R.T.: 0.027 min
Response: 225671
Conc: 1.95 ug/ml

Instrument :
FID_G
ClientSampleId :
S7C(12-20)COMP