

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004531.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 17:30
Operator : AJ\SJ
Sample : K2182-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S8B(2-10)COMP

Integration File: autoint1.e
Quant Time: Apr 02 23:32:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.410	1142008	11.072 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004531.D
Signal(s) : FID1A.ch
Acq On : 02 Apr 2019 17:30
Operator : AJ\SJ
Sample : K2182-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
S8B(2-10)COMP

Integration File: autoint1.e
Quant Time: Apr 02 23:32:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rx1-1ms
Signal Info : 20mx0.18mmx0.18um

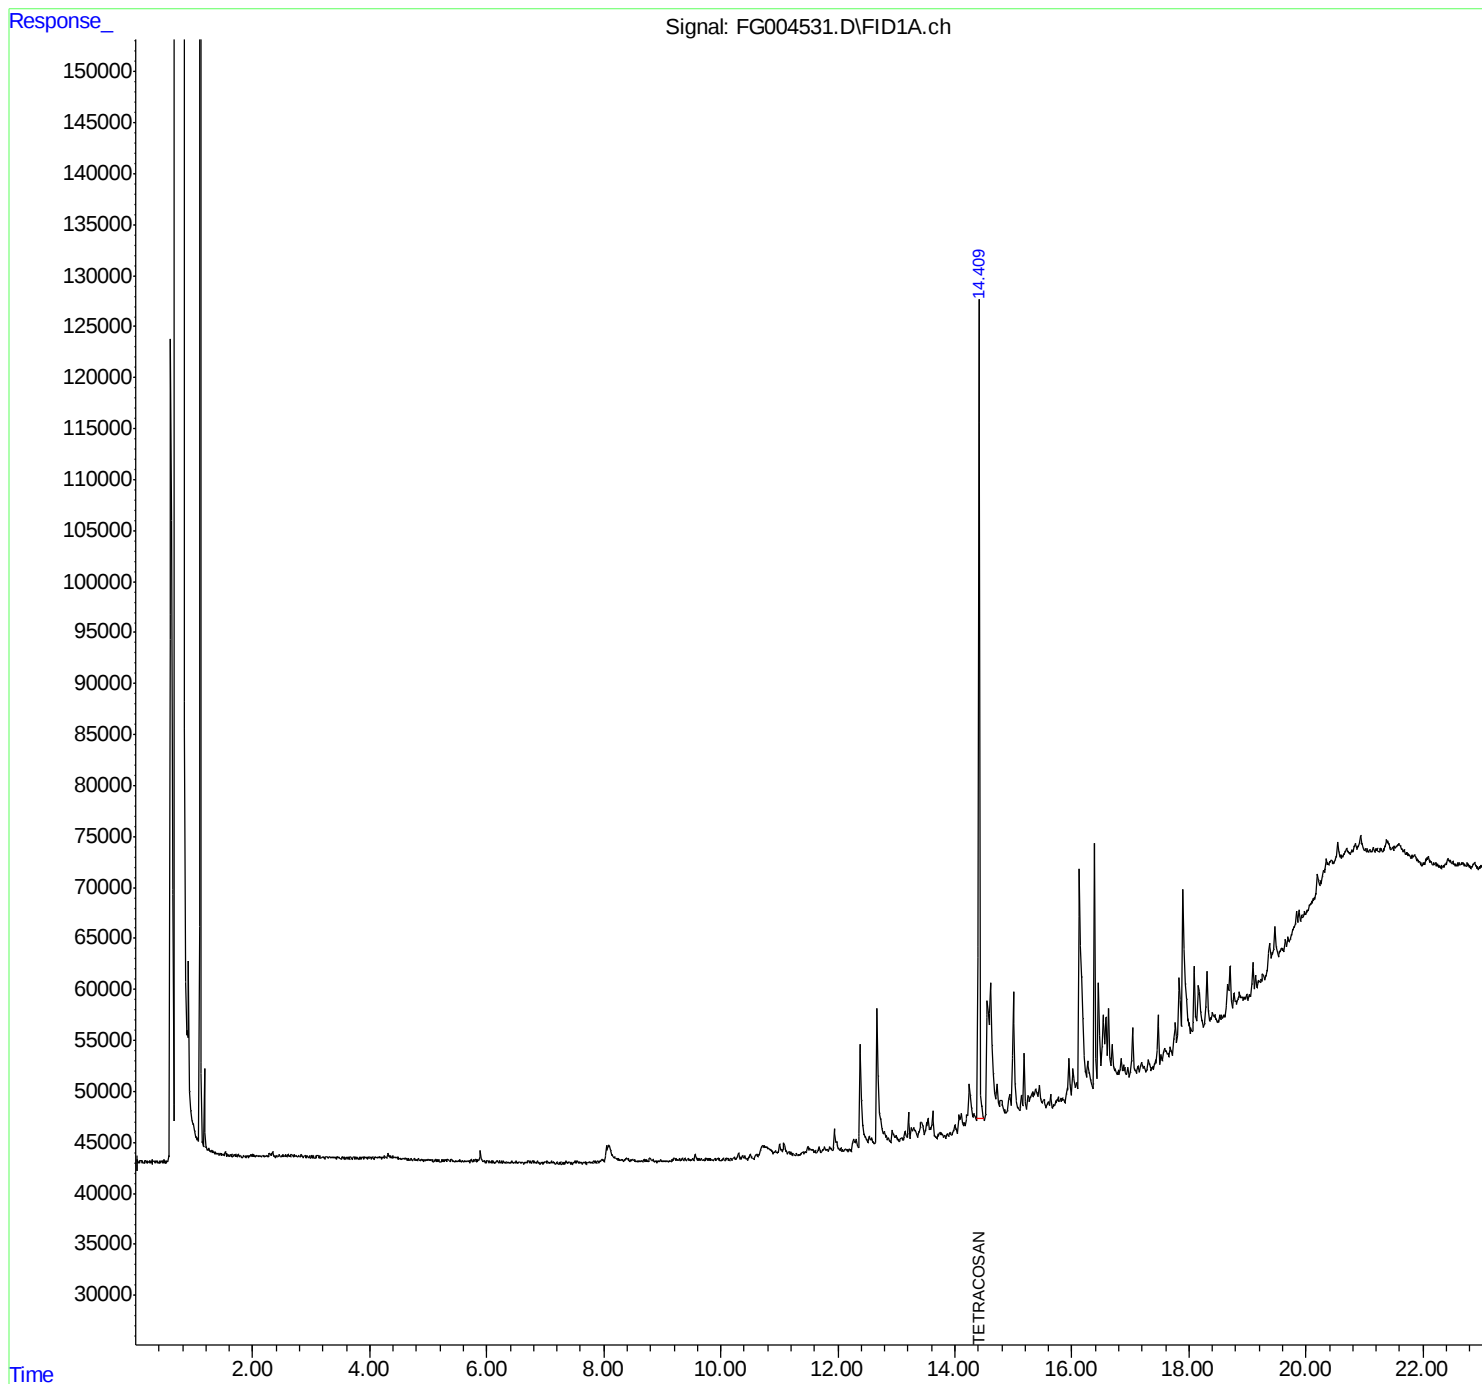

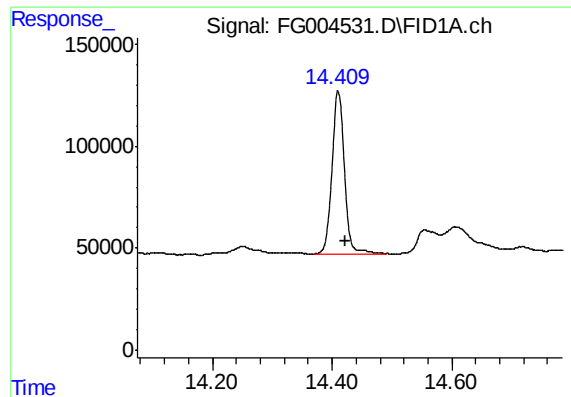

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.410 min
Delta R.T.: -0.012 min
Response: 1142008
Conc: 11.07 ug/ml

Instrument :
FID_G
ClientSampleId :
S8B(2-10)COMP