

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
 Data File : FG004543.D
 Signal(s) : FID1A.ch
 Acq On : 03 Apr 2019 00:13
 Operator : AJ\SJ
 Sample : PB118450BS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB118450BS

Manual Integrations
 APPROVED

Sohil
 4/3/2019 5:58:51 PM

Integration File: autoint1.e
 Quant Time: Apr 03 00:42:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.420	2040835	19.786 ug/ml
Target Compounds			
1) N-OCTANE	2.076	2556707	23.947 ug/ml
2) N-DECANE	4.151	2594206	24.577 ug/ml
3) N-DODECANE	6.174	2591257	24.595 ug/ml
4) N-TETRADECANE	7.967	2587139	23.878 ug/ml
5) N-HEXADECANE	9.569	2550931	22.800 ug/ml
6) N-OCTADECANE	11.010	2494209	21.990 ug/ml
7) N-EICOSANE	12.321	2406831	21.054 ug/ml
8) N-DOCOSANE	13.521	2355062	20.602 ug/ml
10) N-TETRACOSANE	14.623	2338808	20.247 ug/ml
11) N-HEXACOSANE	15.646	2285028	19.933 ug/ml
12) N-OCTACOSANE	16.598	2302763	19.905 ug/ml
13) N-TRIACONTANE	17.486	2327128	19.616 ug/ml
14) N-DOTRIACONTANE	18.319	2321628	19.799 ug/mlm
15) N-TETRATRIACONTANE	19.104	2309480	20.728 ug/mlm
16) N-HEXATRIACONTANE	19.848	2326391	20.870 ug/mlm
17) N-OCTATRIACONTANE	20.560	2085216	20.980 ug/mlm
18) N-TETRACONTANE	21.393	2220005	20.524 ug/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040219\
Data File : FG004543.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 00:13
Operator : AJ\SJ
Sample : PB118450BS
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
FID_G
ClientSampled :
PB118450BS


Manual Integrations
APPROVED

Sohil
4/3/2019 5:58:51 PM

Integration File: autoint1.e
Quant Time: Apr 03 00:42:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

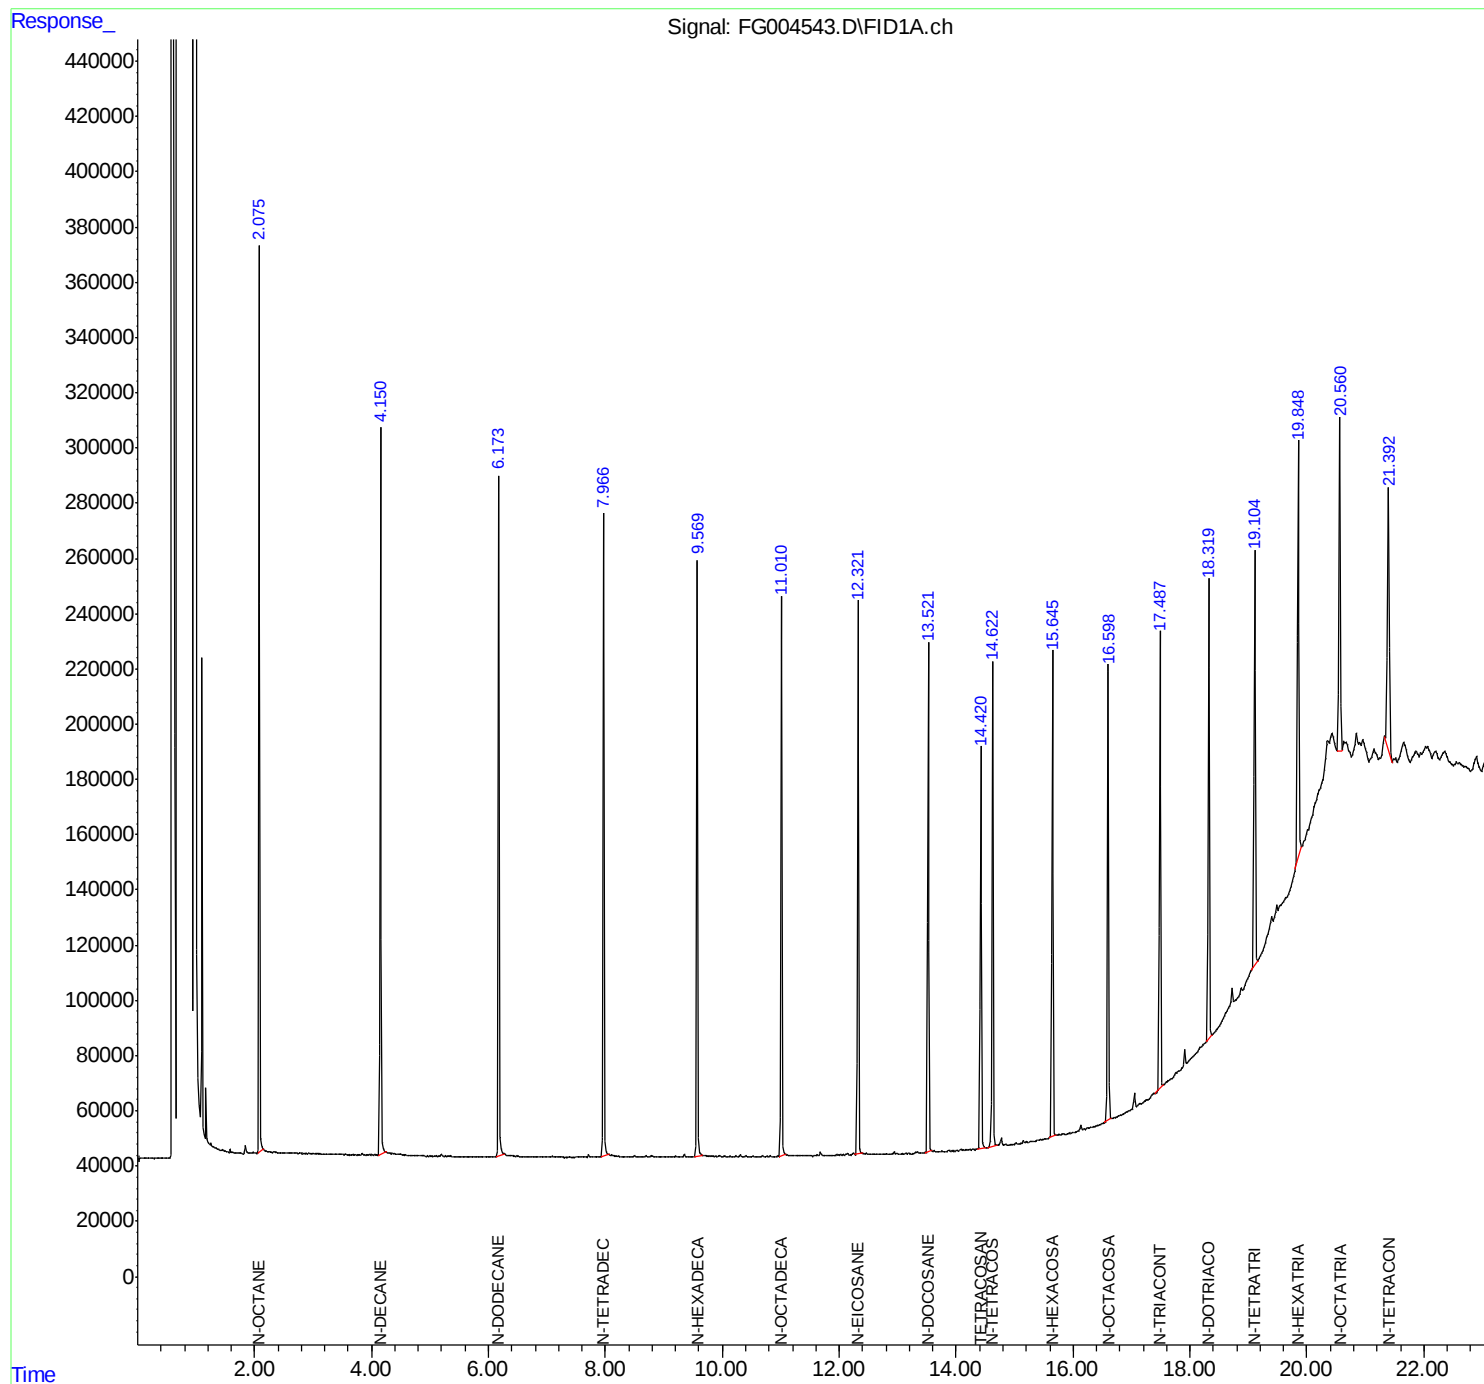

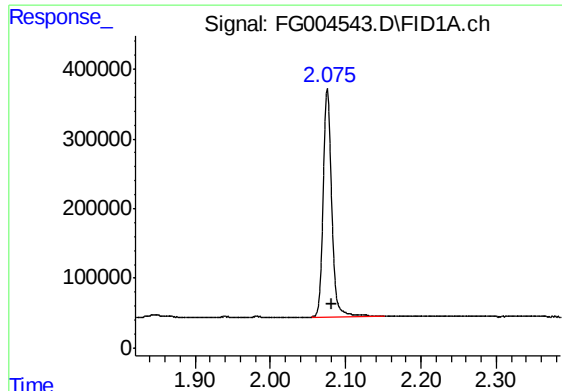


#1 N-OCTANE

R.T.: 2.076 min
Delta R.T.: -0.006 min
Response: 2556707
Conc: 23.95 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118450BS


Manual Integrations
APPROVED

Sohil
4/3/2019 5:58:51 PM

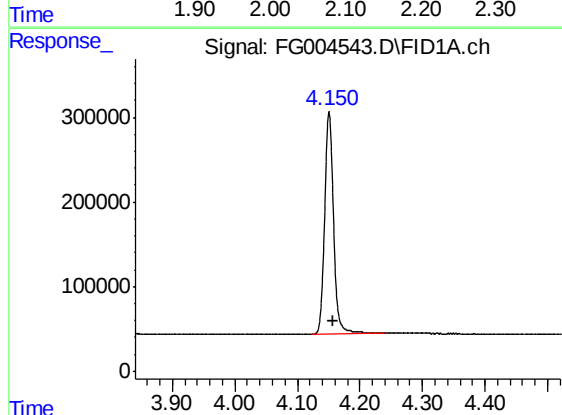


#2 N-DECANE

R.T.: 4.151 min
Delta R.T.: -0.006 min
Response: 2594206
Conc: 24.58 ug/ml

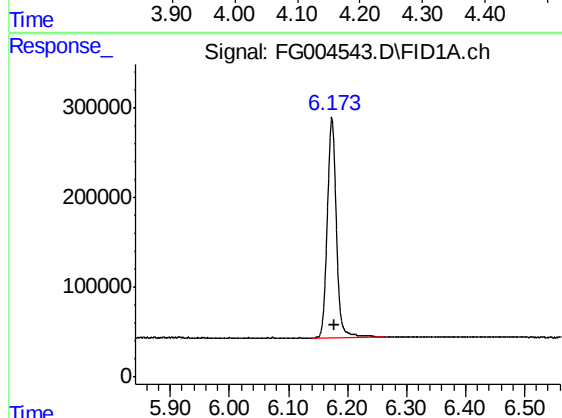


#3 N-DODECANE

R.T.: 6.174 min
Delta R.T.: -0.004 min
Response: 2591257
Conc: 24.59 ug/ml

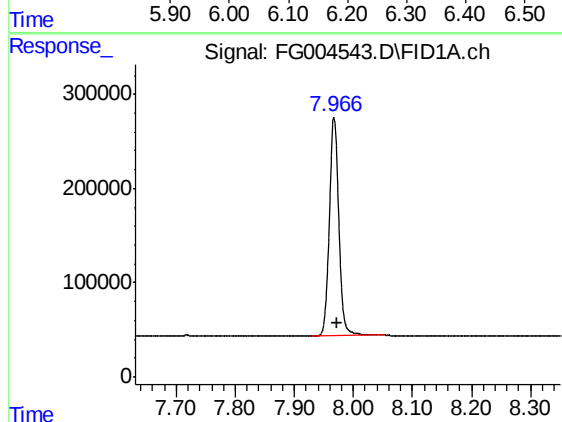

#4 N-TETRADECANE

R.T.: 7.967 min
Delta R.T.: -0.004 min
Response: 2587139
Conc: 23.88 ug/ml

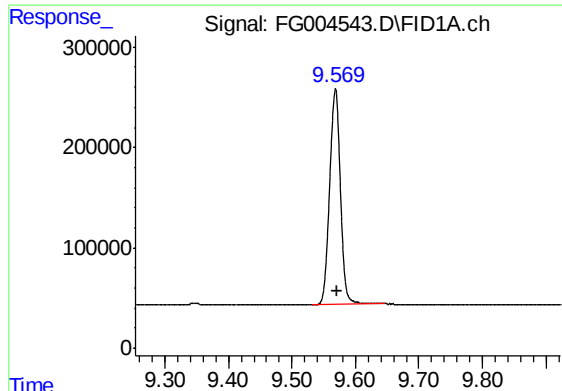


#5 N-HEXADECANE

R.T.: 9.569 min
Delta R.T.: -0.003 min
Response: 2550931
Conc: 22.80 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118450BS


Manual Integrations
APPROVED

Sohil
4/3/2019 5:58:51 PM

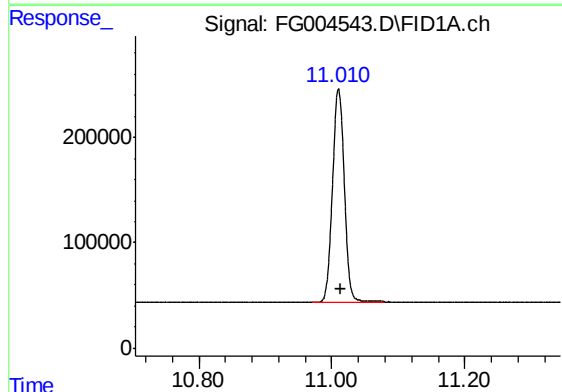


#6 N-OCTADECANE

R.T.: 11.010 min
Delta R.T.: -0.003 min
Response: 2494209
Conc: 21.99 ug/ml

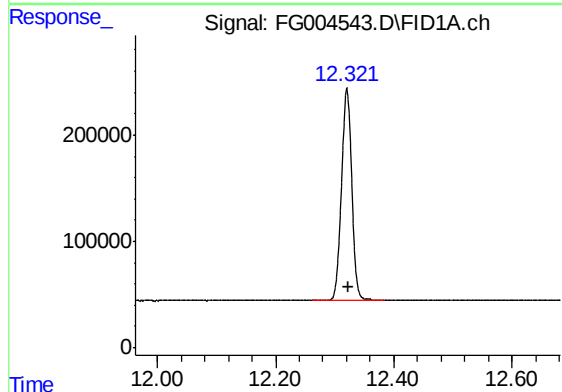


#7 N-EICOSANE

R.T.: 12.321 min
Delta R.T.: -0.002 min
Response: 2406831
Conc: 21.05 ug/ml

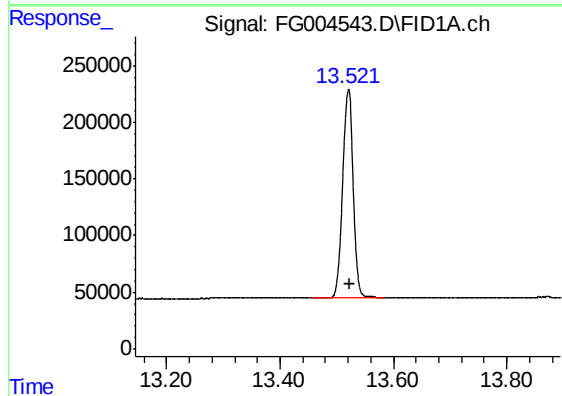

#8 N-DOCOSANE

R.T.: 13.521 min
Delta R.T.: -0.001 min
Response: 2355062
Conc: 20.60 ug/ml

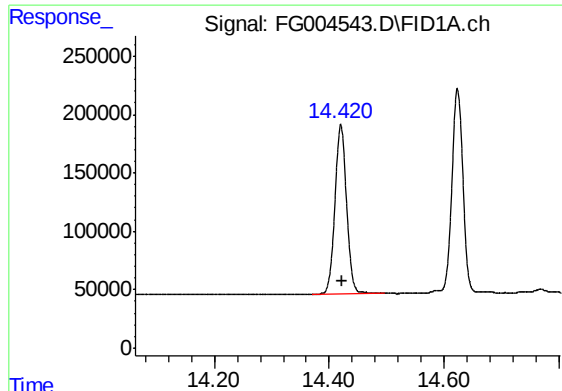


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.420 min
Delta R.T.: -0.002 min
Response: 2040835
Conc: 19.79 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118450BS


Manual Integrations
APPROVED

Sohil
4/3/2019 5:58:51 PM

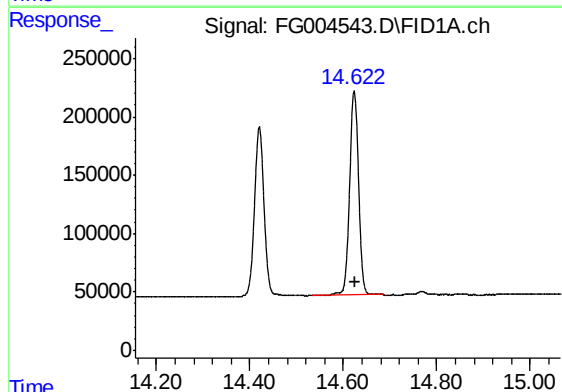


#10 N-TETRACOSANE

R.T.: 14.623 min
Delta R.T.: -0.002 min
Response: 2338808
Conc: 20.25 ug/ml

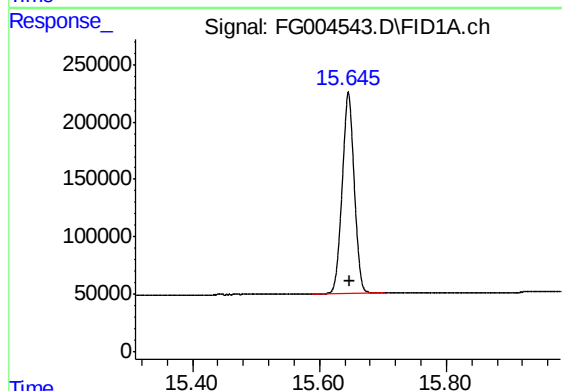


#11 N-HEXACOSANE

R.T.: 15.646 min
Delta R.T.: -0.001 min
Response: 2285028
Conc: 19.93 ug/ml

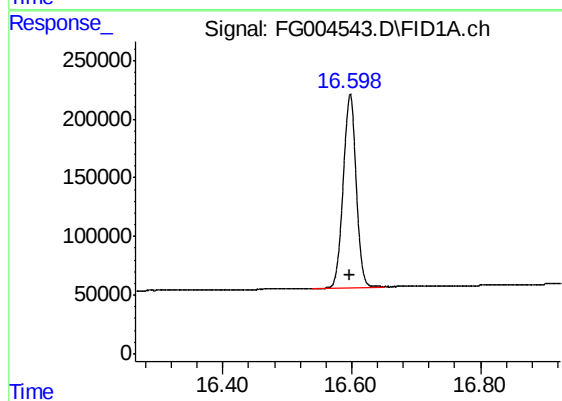

#12 N-OCTACOSANE

R.T.: 16.598 min
Delta R.T.: 0.000 min
Response: 2302763
Conc: 19.90 ug/ml

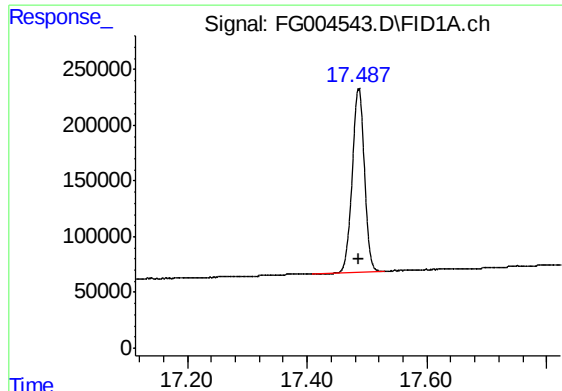


#13 N-TRIACONTANE

R.T.: 17.486 min
Delta R.T.: 0.000 min
Response: 2327128
Conc: 19.62 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118450BS


Manual Integrations
APPROVED

Sohil
4/3/2019 5:58:51 PM

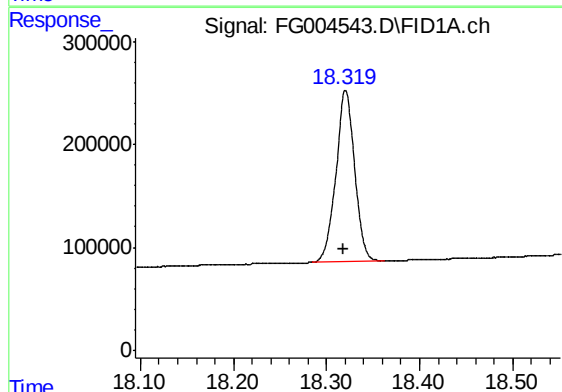


#14 N-DOTRIACONTANE

R.T.: 18.319 min
Delta R.T.: 0.000 min
Response: 2321628
Conc: 19.80 ug/ml m

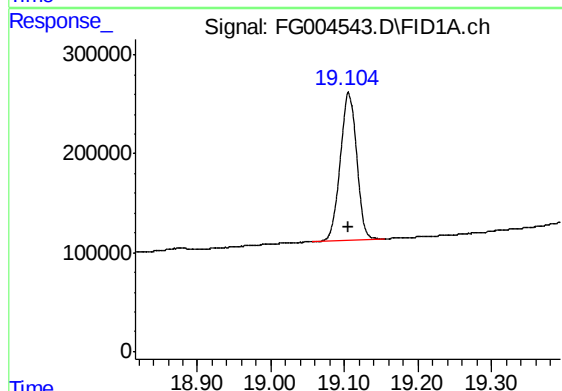


#15 N-TETRATRIACONTANE

R.T.: 19.104 min
Delta R.T.: 0.000 min
Response: 2309480
Conc: 20.73 ug/ml m

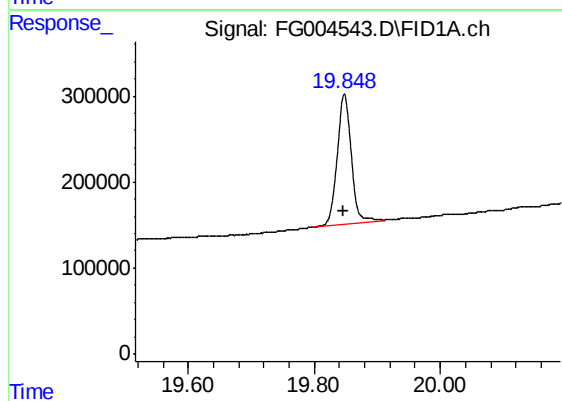

#16 N-HEXATRIACONTANE

R.T.: 19.848 min
Delta R.T.: 0.001 min
Response: 2326391
Conc: 20.87 ug/ml m

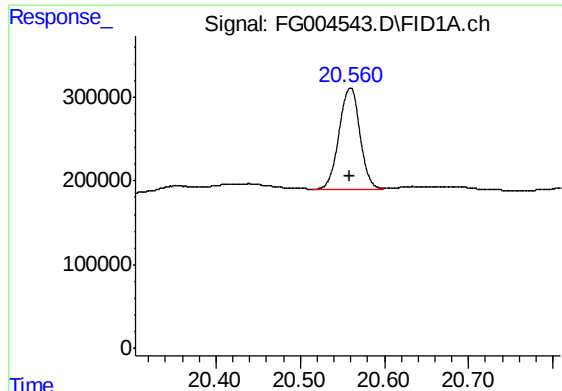


#17 N-OCTATRIACONTANE

R.T.: 20.560 min
Delta R.T.: 0.001 min
Response: 2085216
Conc: 20.98 ug/ml m

Instrument :
FID_G
ClientSampleId :
PB118450BS

Manual Integrations
APPROVED

Sohil
4/3/2019 5:58:51 PM

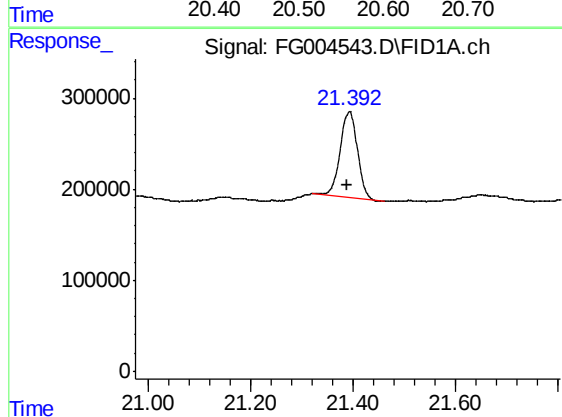

#18 N-TETRACONTANE

R.T.: 21.393 min
Delta R.T.: 0.004 min
Response: 2220005
Conc: 20.52 ug/ml