

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
Data File : FG004551.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 12:58
Operator : AJ\SJ
Sample : K2178-02 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
COMP-17

Integration File: autoint1.e
Quant Time: Apr 03 14:35:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.489	134192	1.131 ug/ml
14) N-DOTRIACONTANE	18.321	14967	0.128 ug/ml
15) N-TETRATRIACONTANE	19.103	207988	1.867 ug/ml
16) N-HEXATRIACONTANE	19.843	99287	0.891 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
Data File : FG004551.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 12:58
Operator : AJ\SJ
Sample : K2178-02 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
COMP-17

Integration File: autoint1.e
Quant Time: Apr 03 14:35:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

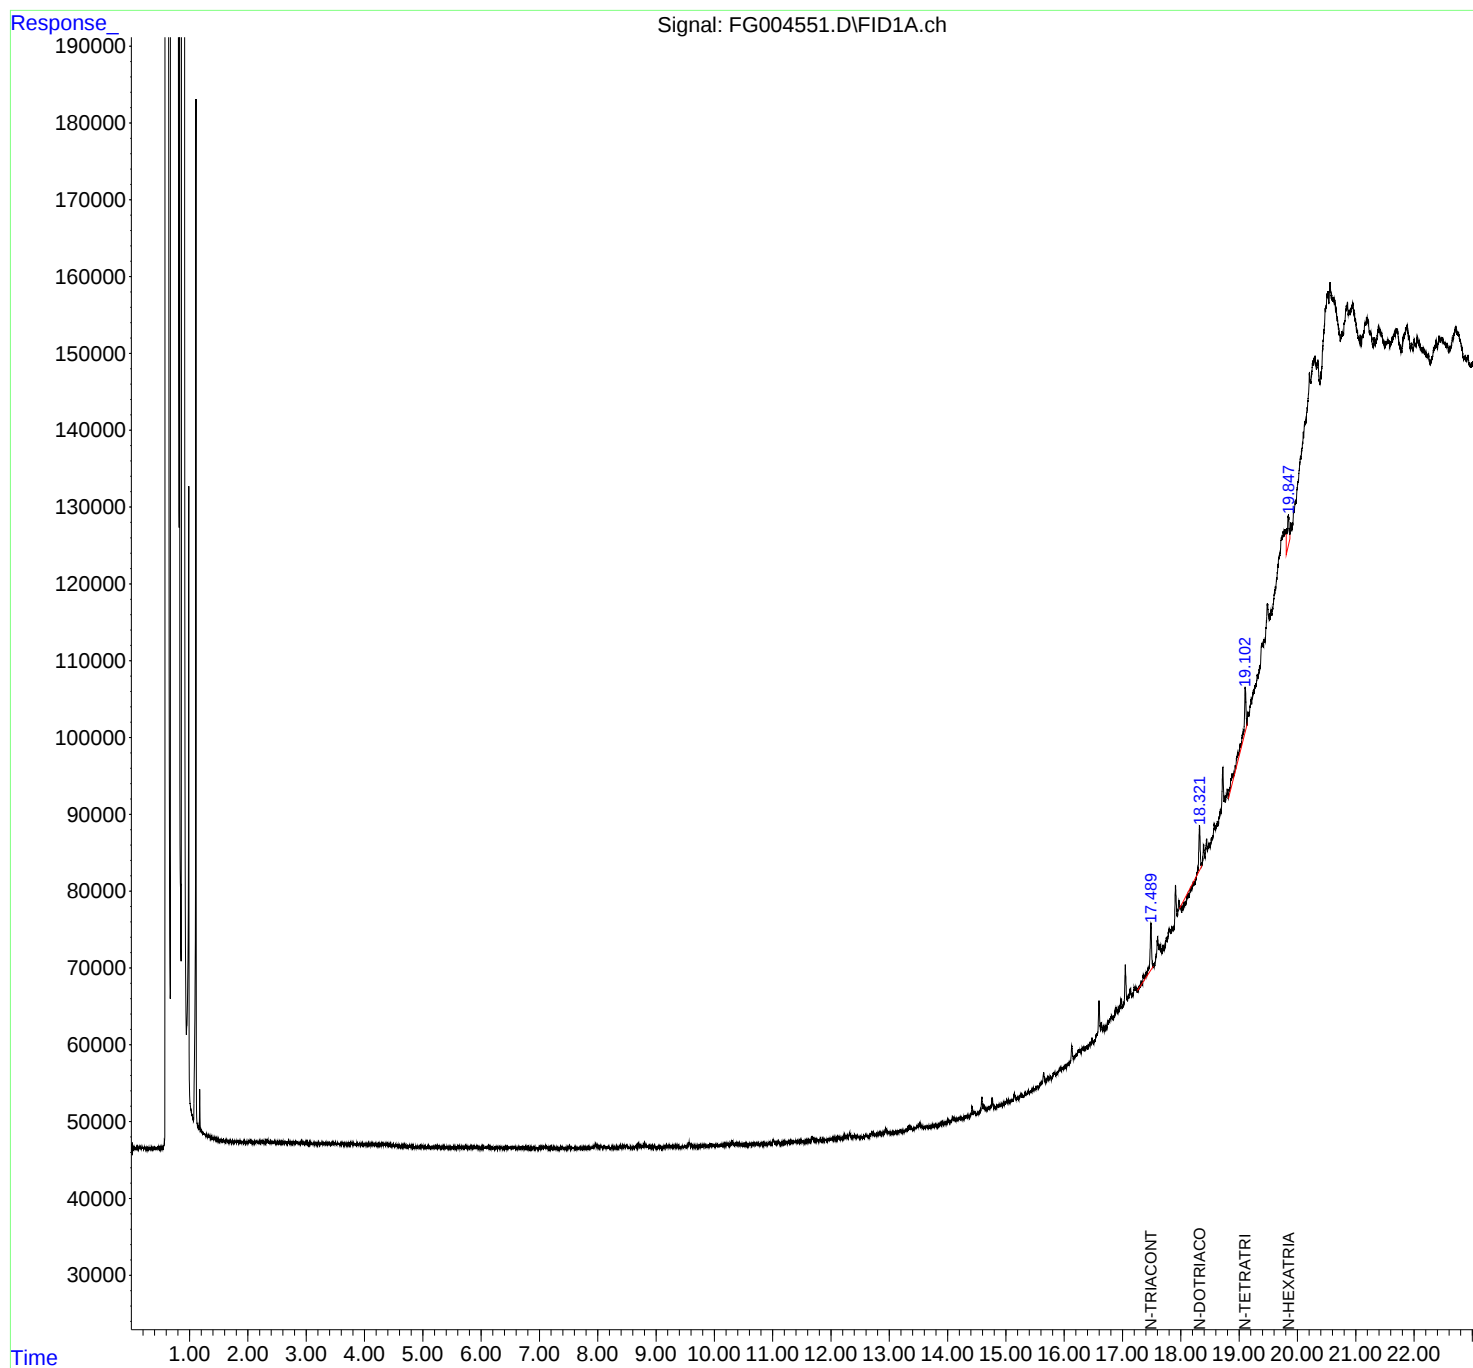


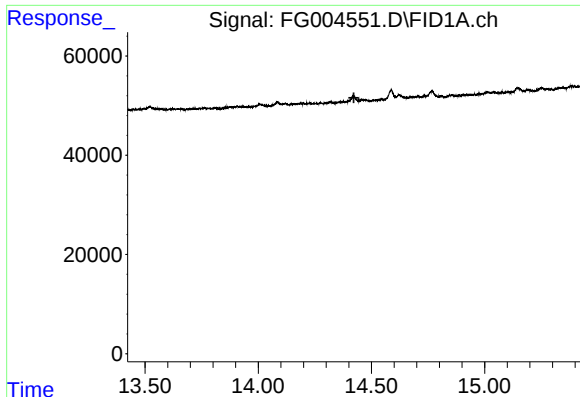

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.422 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
COMP-17

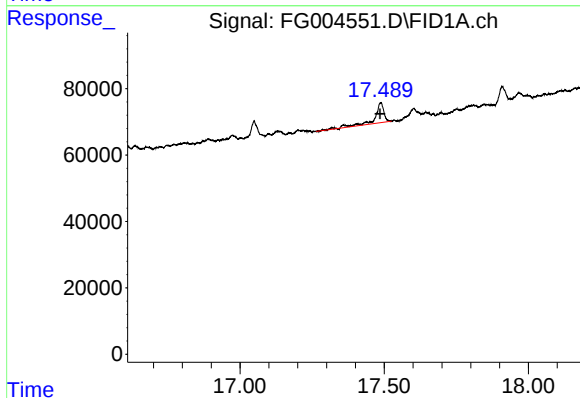


#13 N-TRIACONTANE

R.T.: 17.489 min
Delta R.T.: 0.003 min
Response: 134192
Conc: 1.13 ug/ml

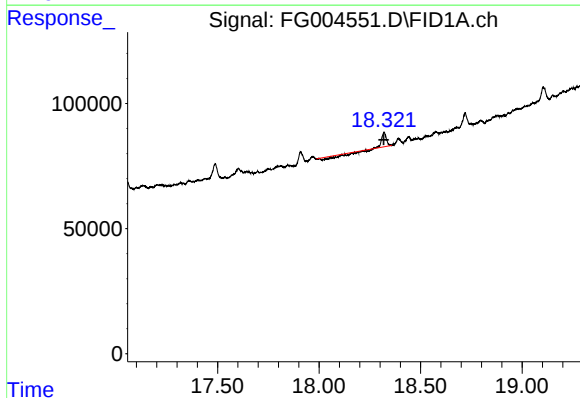


#14 N-DOTRIACONTANE

R.T.: 18.321 min
Delta R.T.: 0.002 min
Response: 14967
Conc: 0.13 ug/ml

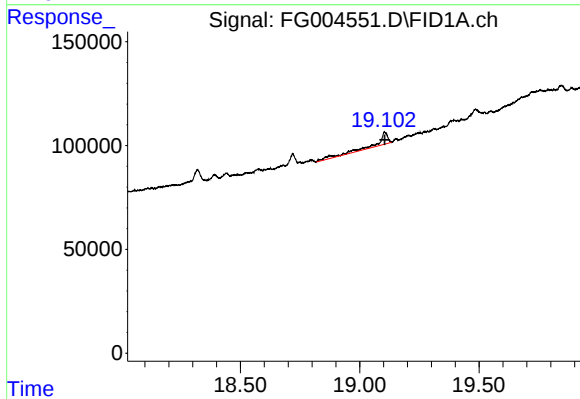

#15 N-TETRATRIACONTANE

R.T.: 19.103 min
Delta R.T.: -0.002 min
Response: 207988
Conc: 1.87 ug/ml

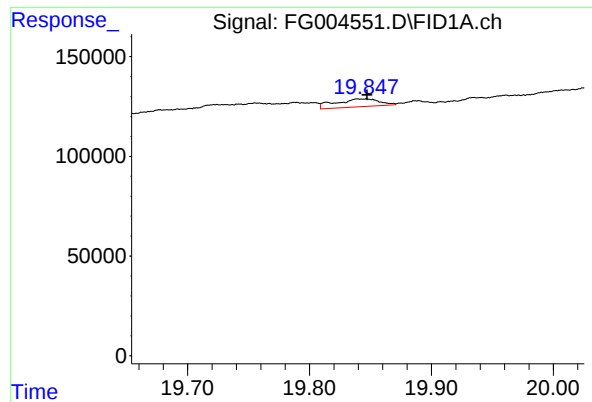

#16 N-HEXATRIACONTANE

R.T.: 19.843 min
Delta R.T.: -0.004 min
Response: 99287
Conc: 0.89 ug/ml

Instrument :
FID_G
ClientSampleId :
COMP-17