

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
 Data File : FG004560.D
 Signal(s) : FID1A.ch
 Acq On : 03 Apr 2019 17:39
 Operator : AJ\SJ
 Sample : K2176-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 QNWP8-MW24D-GW

Integration File: autoint1.e
 Quant Time: Apr 04 03:20:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.417	1818069	17.626 ug/ml
Target Compounds			
3) N-DODECANE	6.129	222136	2.108 ug/ml
4) N-TETRADECANE	8.033f	94491	0.872 ug/ml
7) N-EICOSANE	12.377f	271853	2.378 ug/ml
12) N-OCTACOSANE	16.593	123515	1.068 ug/ml
13) N-TRIACONTANE	17.483	172201	1.452 ug/ml
14) N-DOTRIACONTANE	18.314	159342	1.359 ug/ml
16) N-HEXATRIACONTANE	19.884	16443	0.148 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
Data File : FG004560.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 17:39
Operator : AJ\SJ
Sample : K2176-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
QNWP8-MW24D-GW

Integration File: autoint1.e
Quant Time: Apr 04 03:20:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

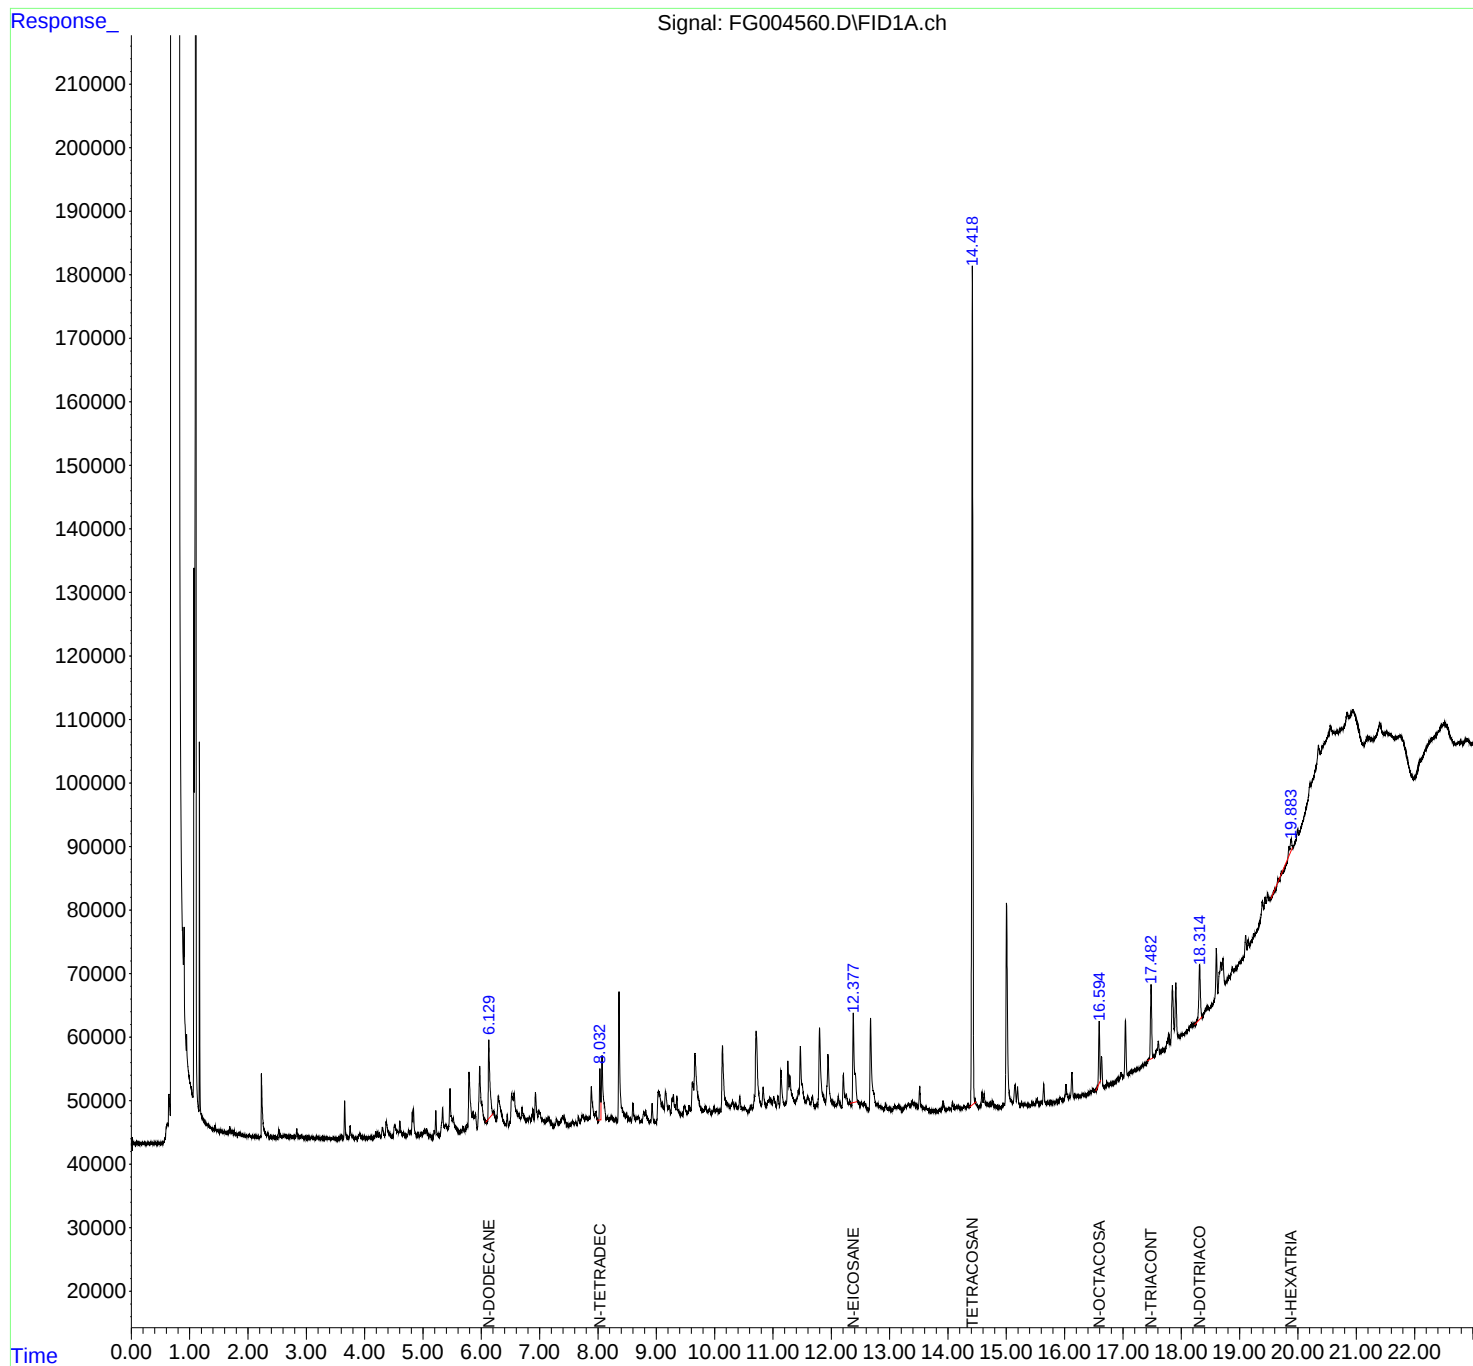


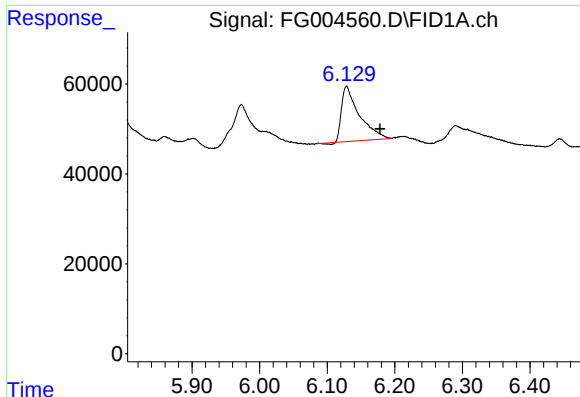

#3 N-DODECANE


R.T.: 6.129 min
Delta R.T.: -0.049 min
Response: 222136
Conc: 2.11 ug/ml

Instrument :
FID_G
ClientSampleId :
QNWP8-MW24D-GW

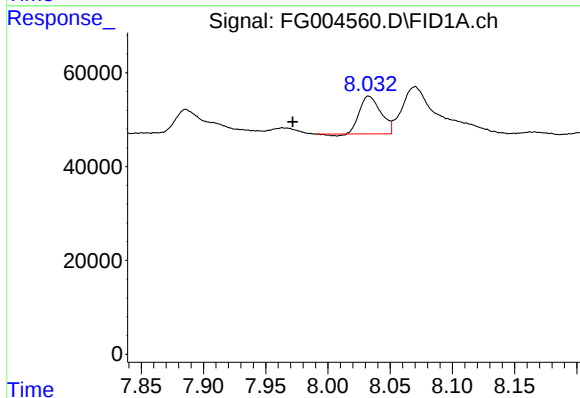


#4 N-TETRADECANE

R.T.: 8.033 min
Delta R.T.: 0.061 min
Response: 94491
Conc: 0.87 ug/ml

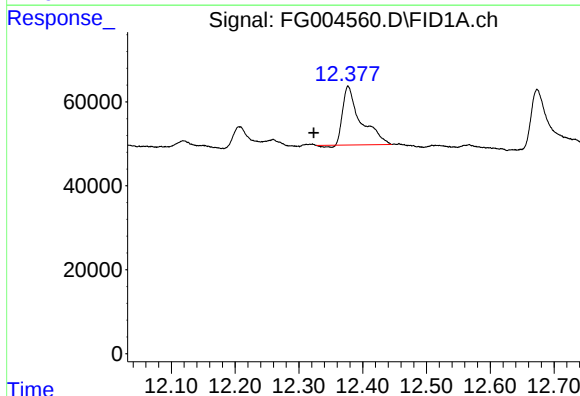


#7 N-EICOSANE

R.T.: 12.377 min
Delta R.T.: 0.054 min
Response: 271853
Conc: 2.38 ug/ml

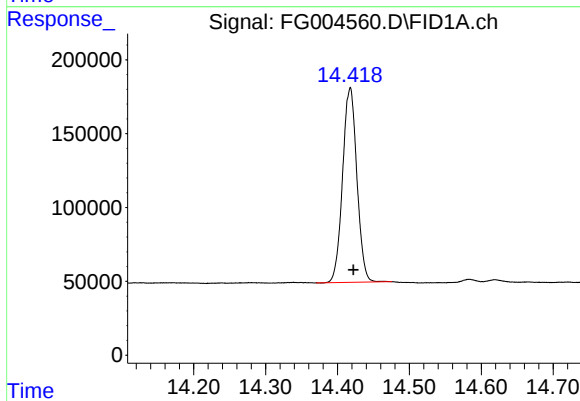

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.417 min
Delta R.T.: -0.005 min
Response: 1818069
Conc: 17.63 ug/ml

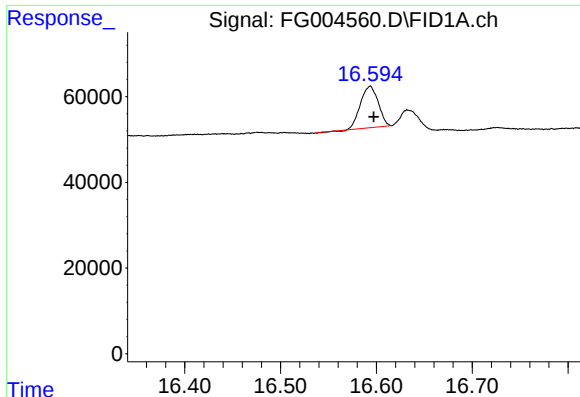

#12 N-OCTACOSANE


R.T.: 16.593 min
Delta R.T.: -0.004 min
Response: 123515
Conc: 1.07 ug/ml

Instrument :
FID_G
ClientSampleId :
QNWP8-MW24D-GW

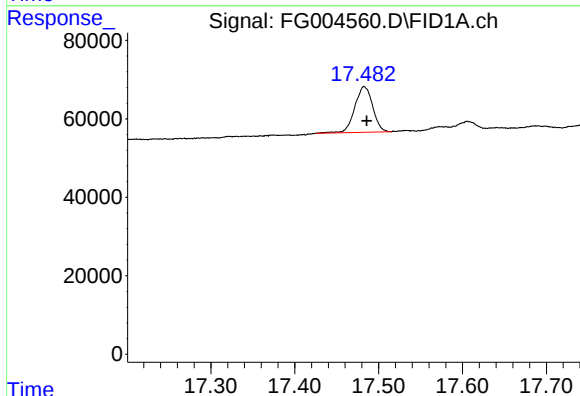


#13 N-TRIACONTANE

R.T.: 17.483 min
Delta R.T.: -0.003 min
Response: 172201
Conc: 1.45 ug/ml

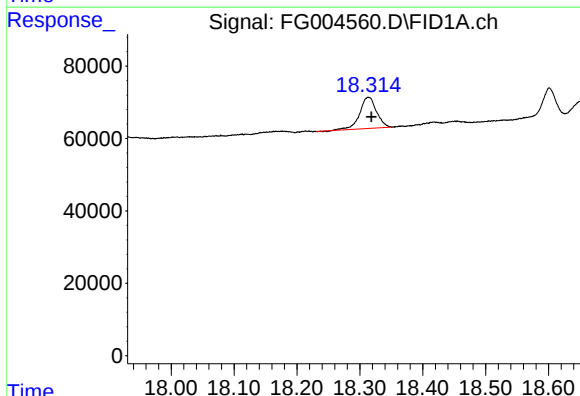

#14 N-DOTRIACONTANE

R.T.: 18.314 min
Delta R.T.: -0.005 min
Response: 159342
Conc: 1.36 ug/ml

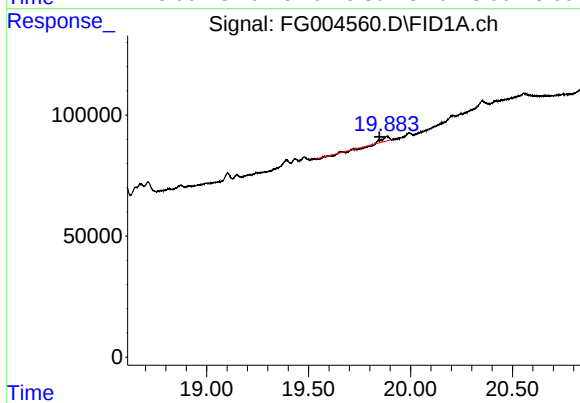

#16 N-HEXATRIACONTANE

R.T.: 19.884 min
Delta R.T.: 0.037 min
Response: 16443
Conc: 0.15 ug/ml