

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
Data File : FG004563.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 19:13
Operator : AJ\SJ
Sample : K2197-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CL-02-040219-A

Integration File: autoint1.e
Quant Time: Apr 04 03:21:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.417	148730	1.442 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.594	142136	1.229 ug/ml
13) N-TRIACONTANE	17.484	131433	1.108 ug/ml
14) N-DOTRIACONTANE	18.318	143689	1.225 ug/ml
15) N-TETRATRIACONTANE	19.103	81798	0.734 ug/ml
16) N-HEXATRIACONTANE	19.850	83356	0.748 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
Data File : FG004563.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 19:13
Operator : AJ\SJ
Sample : K2197-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CL-02-040219-A

Integration File: autoint1.e
Quant Time: Apr 04 03:21:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

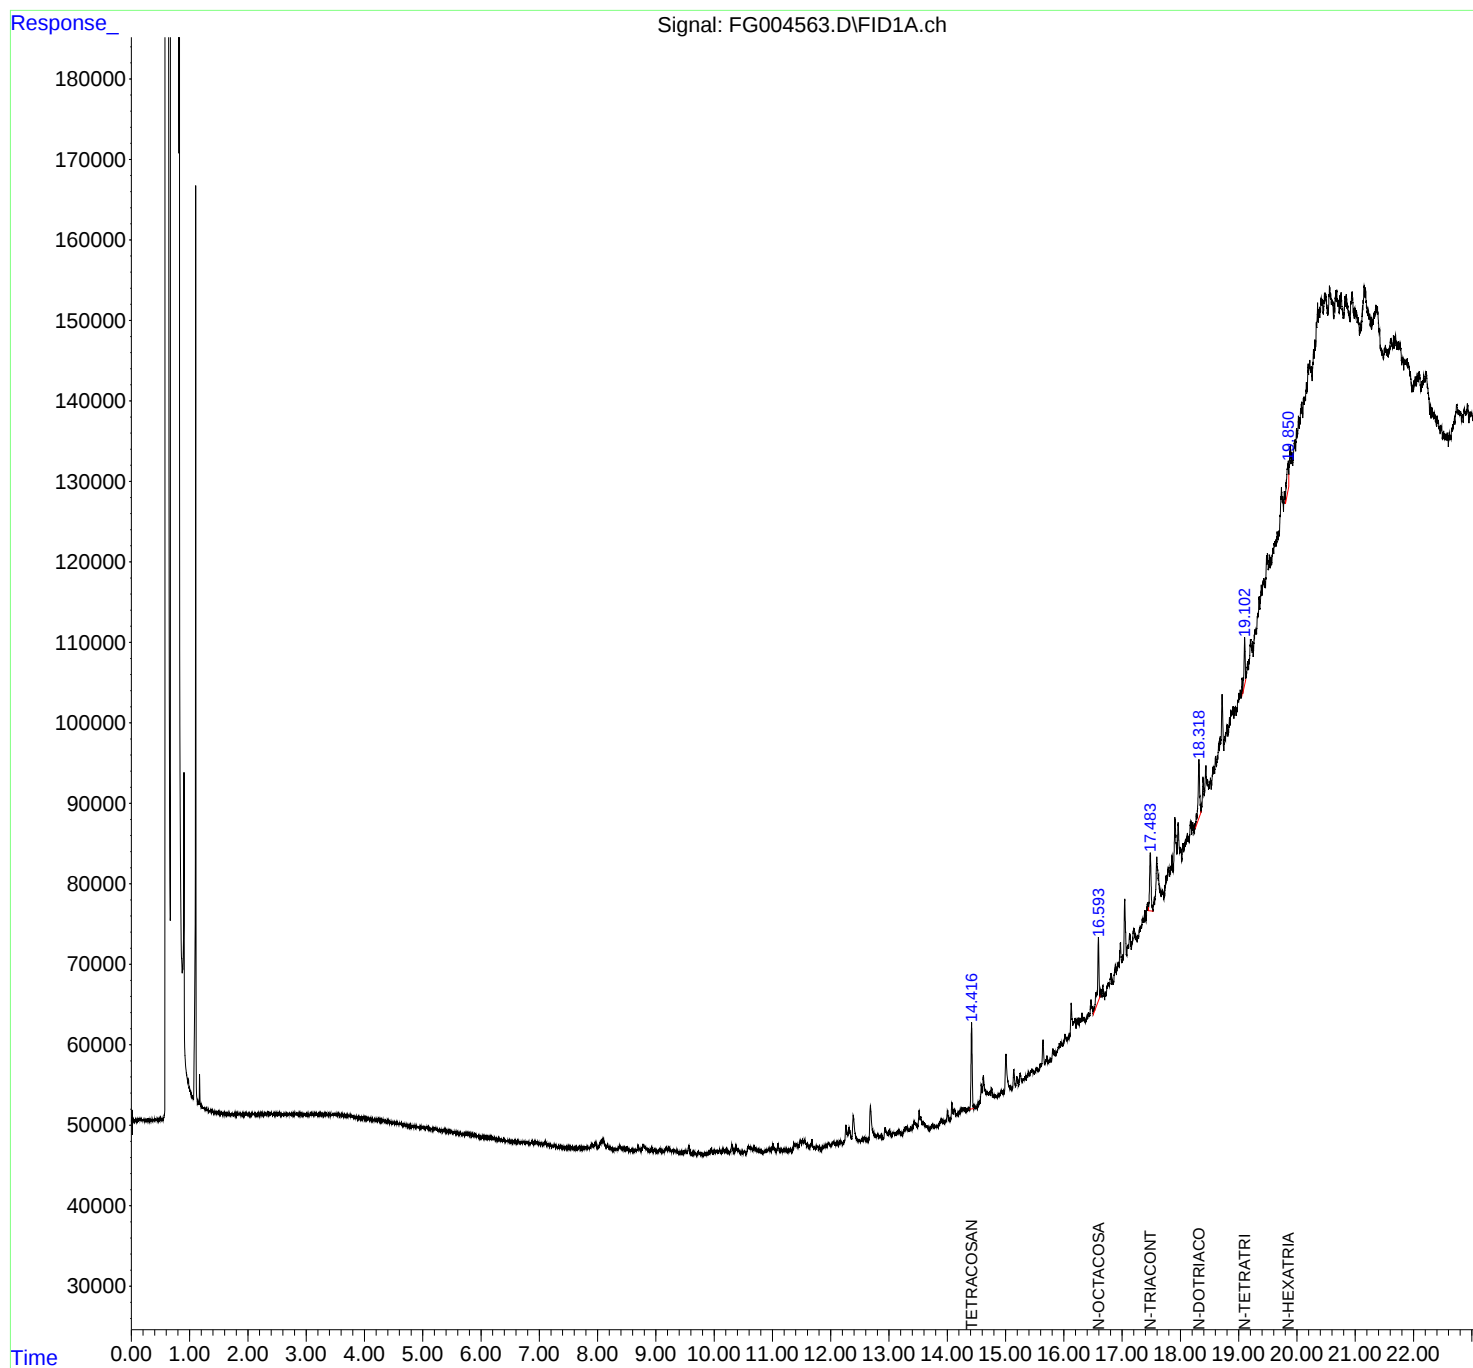


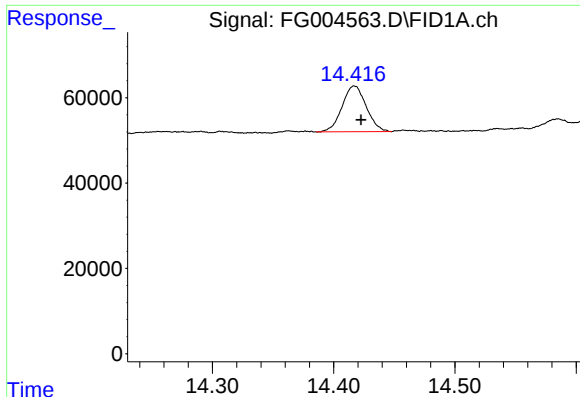

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.417 min
Delta R.T.: -0.005 min
Response: 148730
Conc: 1.44 ug/ml

Instrument :
FID_G
ClientSampleId :
CL-02-040219-A

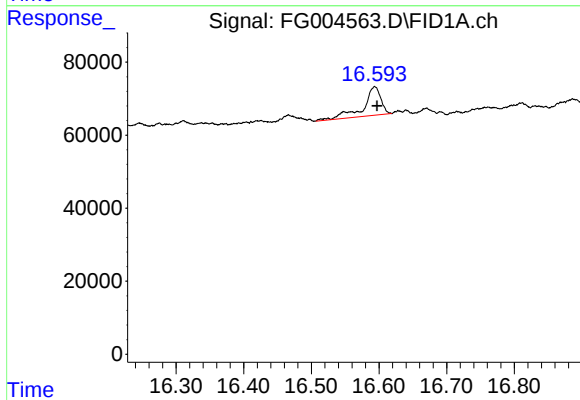


#12 N-OCTACOSANE

R.T.: 16.594 min
Delta R.T.: -0.004 min
Response: 142136
Conc: 1.23 ug/ml

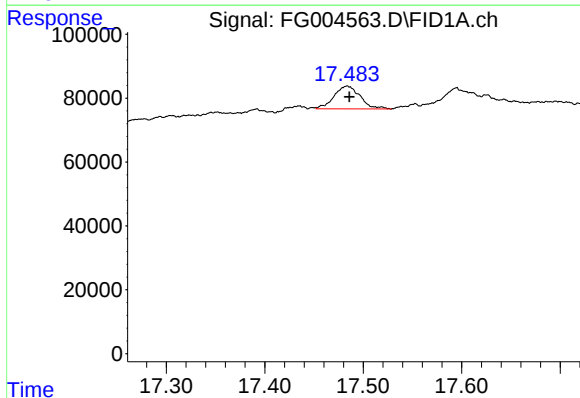


#13 N-TRIACONTANE

R.T.: 17.484 min
Delta R.T.: -0.002 min
Response: 131433
Conc: 1.11 ug/ml

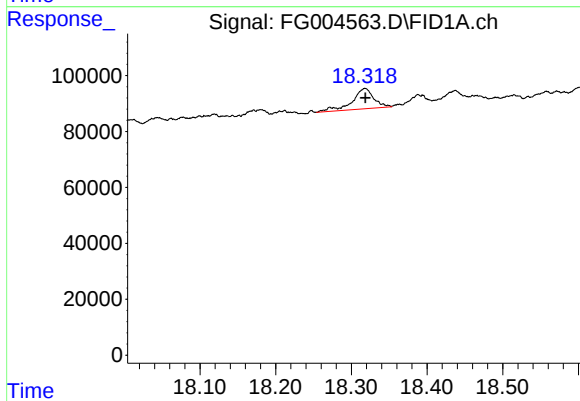

#14 N-DOTRIACONTANE


R.T.: 18.318 min
Delta R.T.: 0.000 min
Response: 143689
Conc: 1.23 ug/ml

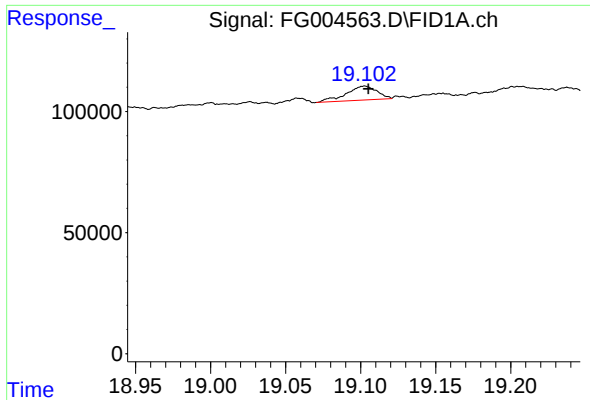

#15 N-TETRATRIACONTANE

R.T.: 19.103 min
Delta R.T.: -0.003 min
Response: 81798
Conc: 0.73 ug/ml

Instrument :
FID_G
ClientSampleId :
CL-02-040219-A

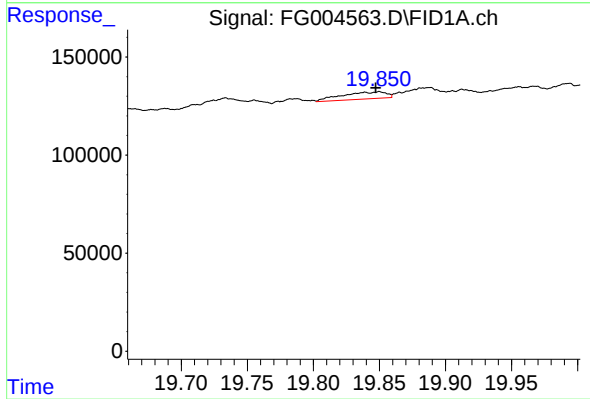

#16 N-HEXATRIACONTANE

R.T.: 19.850 min
Delta R.T.: 0.003 min
Response: 83356
Conc: 0.75 ug/ml