

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
 Data File : FG004564.D
 Signal(s) : FID1A.ch
 Acq On : 03 Apr 2019 19:44
 Operator : AJ\SJ
 Sample : K2199-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 OR-02-040219-A

Integration File: autoint1.e
 Quant Time: Apr 04 03:21:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.416	134918	1.308 ug/ml
Target Compounds			
7) N-EICOSANE	12.380f	319734	2.797 ug/ml
10) N-TETRACOSANE	14.619	245975	2.129 ug/ml
12) N-OCTACOSANE	16.592	99610	0.861 ug/ml
13) N-TRIACONTANE	17.482	168730	1.422 ug/ml
14) N-DOTRIACONTANE	18.317	152945	1.304 ug/ml
15) N-TETRATRIACONTANE	19.101	150634	1.352 ug/ml
16) N-HEXATRIACONTANE	19.846	87279	0.783 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
Data File : FG004564.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 19:44
Operator : AJ\SJ
Sample : K2199-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OR-02-040219-A

Integration File: autoint1.e
Quant Time: Apr 04 03:21:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

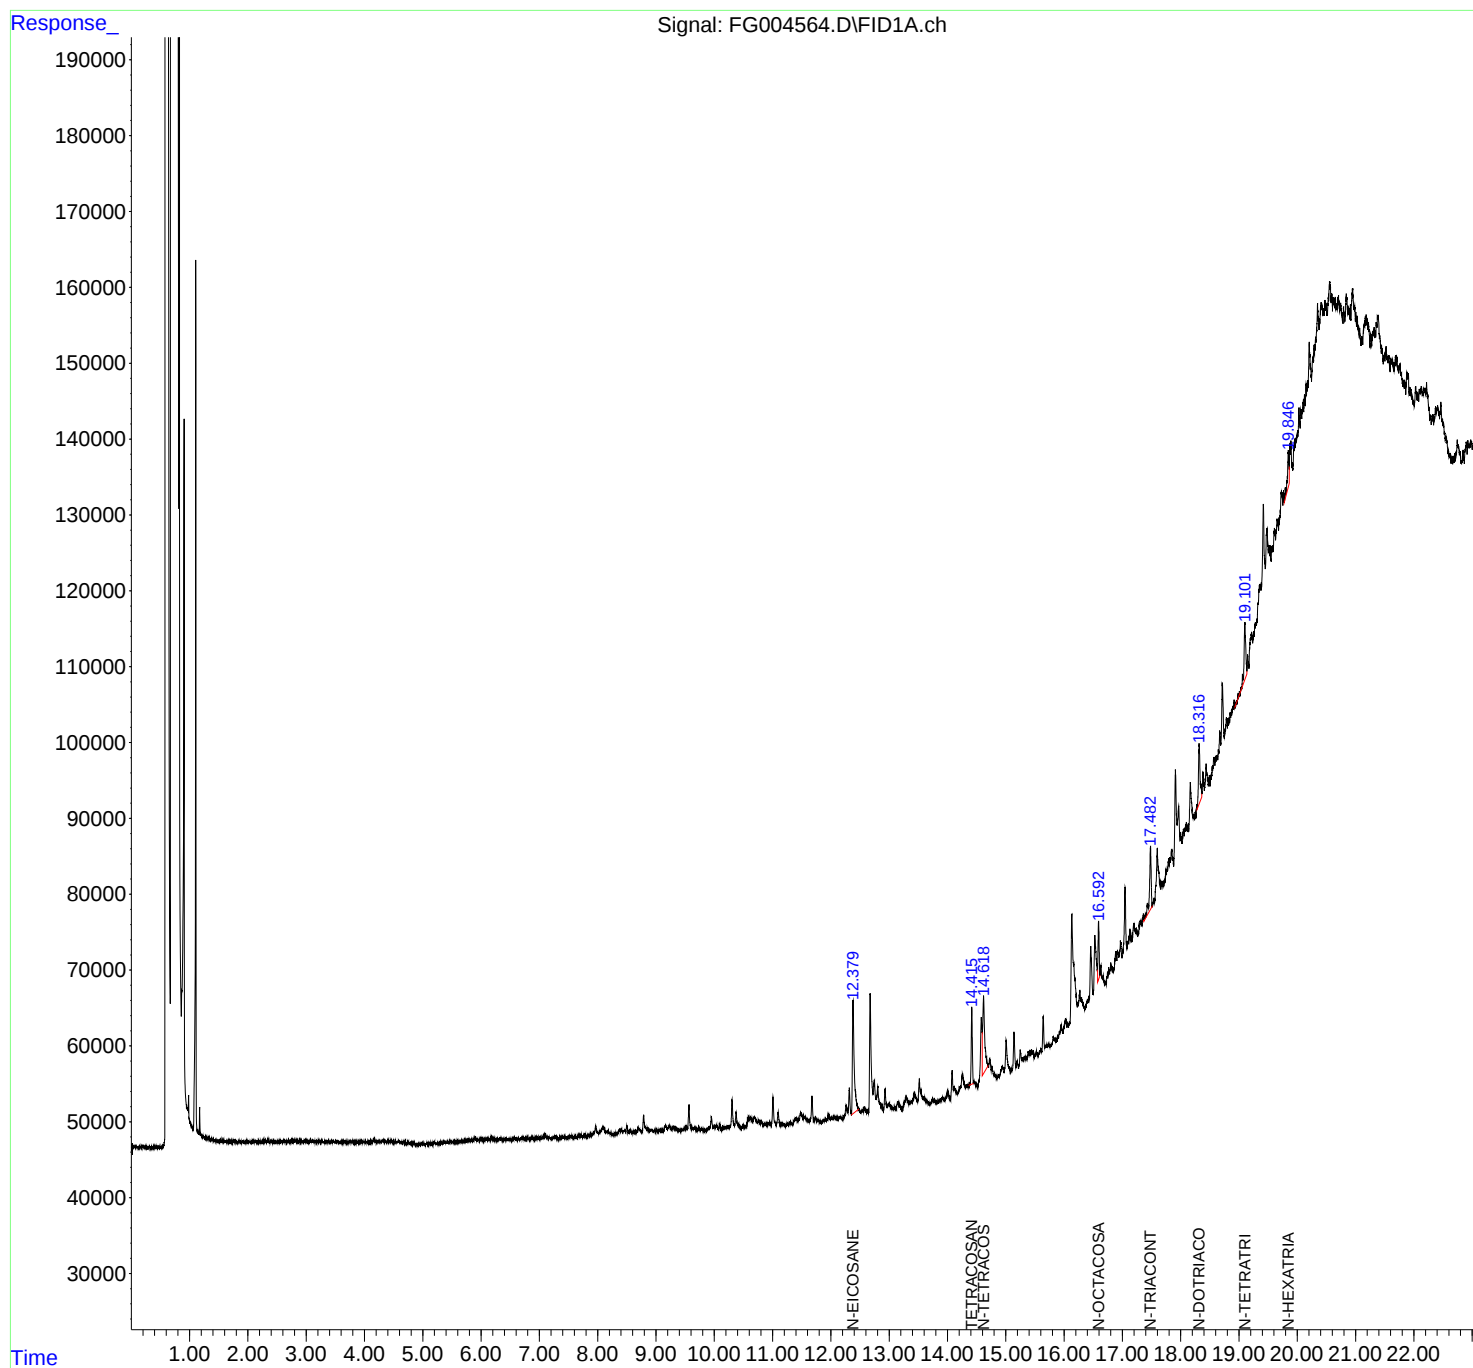


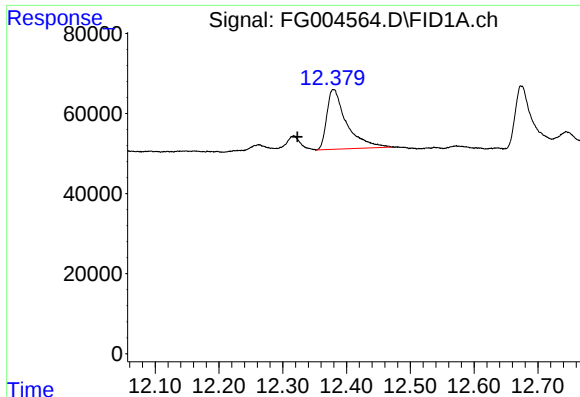

#7 N-EICOSANE


R.T.: 12.380 min
Delta R.T.: 0.057 min
Response: 319734
Conc: 2.80 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-02-040219-A

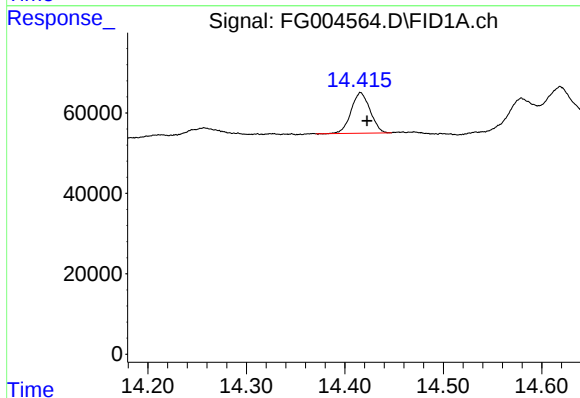


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.416 min
Delta R.T.: -0.006 min
Response: 134918
Conc: 1.31 ug/ml

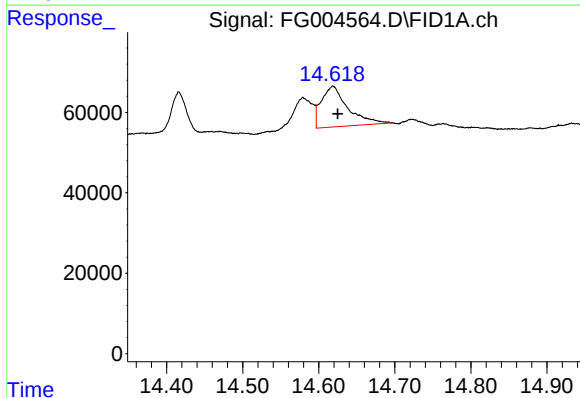


#10 N-TETRACOSANE

R.T.: 14.619 min
Delta R.T.: -0.006 min
Response: 245975
Conc: 2.13 ug/ml

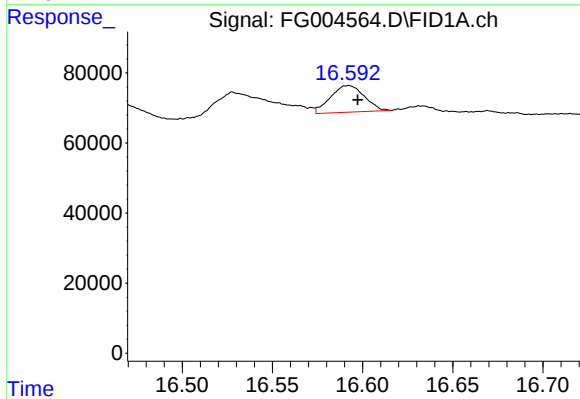

#12 N-OCTACOSANE


R.T.: 16.592 min
Delta R.T.: -0.005 min
Response: 99610
Conc: 0.86 ug/ml

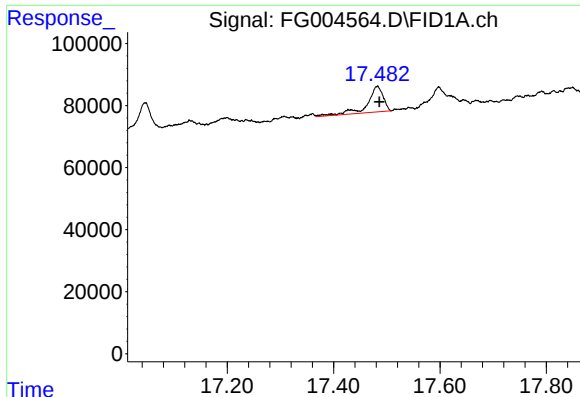

#13 N-TRIACONTANE


R.T.: 17.482 min
Delta R.T.: -0.004 min
Response: 168730
Conc: 1.42 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-02-040219-A

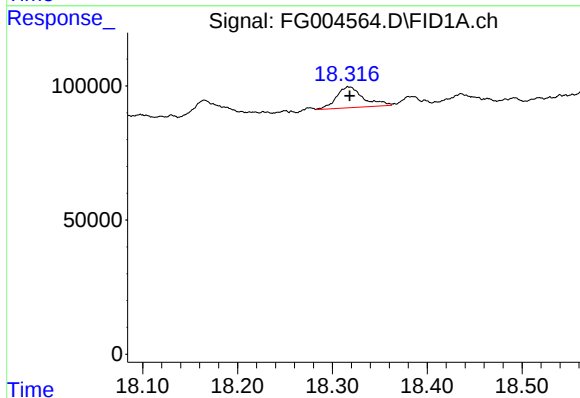


#14 N-DOTRIACONTANE

R.T.: 18.317 min
Delta R.T.: -0.001 min
Response: 152945
Conc: 1.30 ug/ml

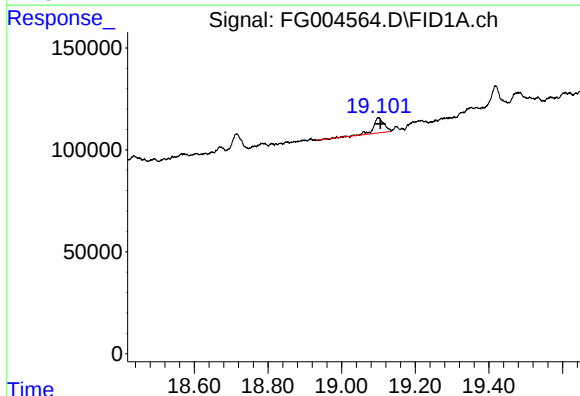

#15 N-TETRATRIACONTANE

R.T.: 19.101 min
Delta R.T.: -0.004 min
Response: 150634
Conc: 1.35 ug/ml

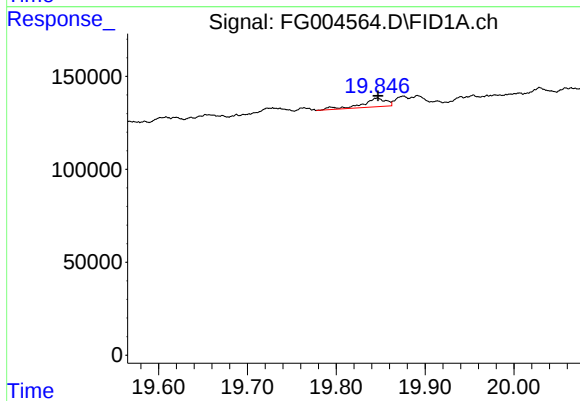

#16 N-HEXATRIACONTANE

R.T.: 19.846 min
Delta R.T.: -0.001 min
Response: 87279
Conc: 0.78 ug/ml