

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
 Data File : FG004567.D
 Signal(s) : FID1A.ch
 Acq On : 03 Apr 2019 21:17
 Operator : AJ\SJ
 Sample : K2203-03 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SU-03-040219-B

Integration File: autoint1.e
 Quant Time: Apr 04 03:22:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.417	140112	1.358 ug/ml
Target Compounds			
7) N-EICOSANE	12.372	800425	7.002 ug/ml
10) N-TETRACOSANE	14.607	544014	4.709 ug/ml
12) N-OCTACOSANE	16.593	130088	1.124 ug/ml
13) N-TRIACONTANE	17.482	225875	1.904 ug/ml
14) N-DOTRIACONTANE	18.322	462547	3.945 ug/ml
15) N-TETRATRIACONTANE	19.103	88148	0.791 ug/ml
16) N-HEXATRIACONTANE	19.881	1066745	9.570 ug/ml
18) N-TETRACONTANE	21.410	1761800	16.288 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040319\
Data File : FG004567.D
Signal(s) : FID1A.ch
Acq On : 03 Apr 2019 21:17
Operator : AJ\SJ
Sample : K2203-03 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SU-03-040219-B

Integration File: autoint1.e
Quant Time: Apr 04 03:22:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

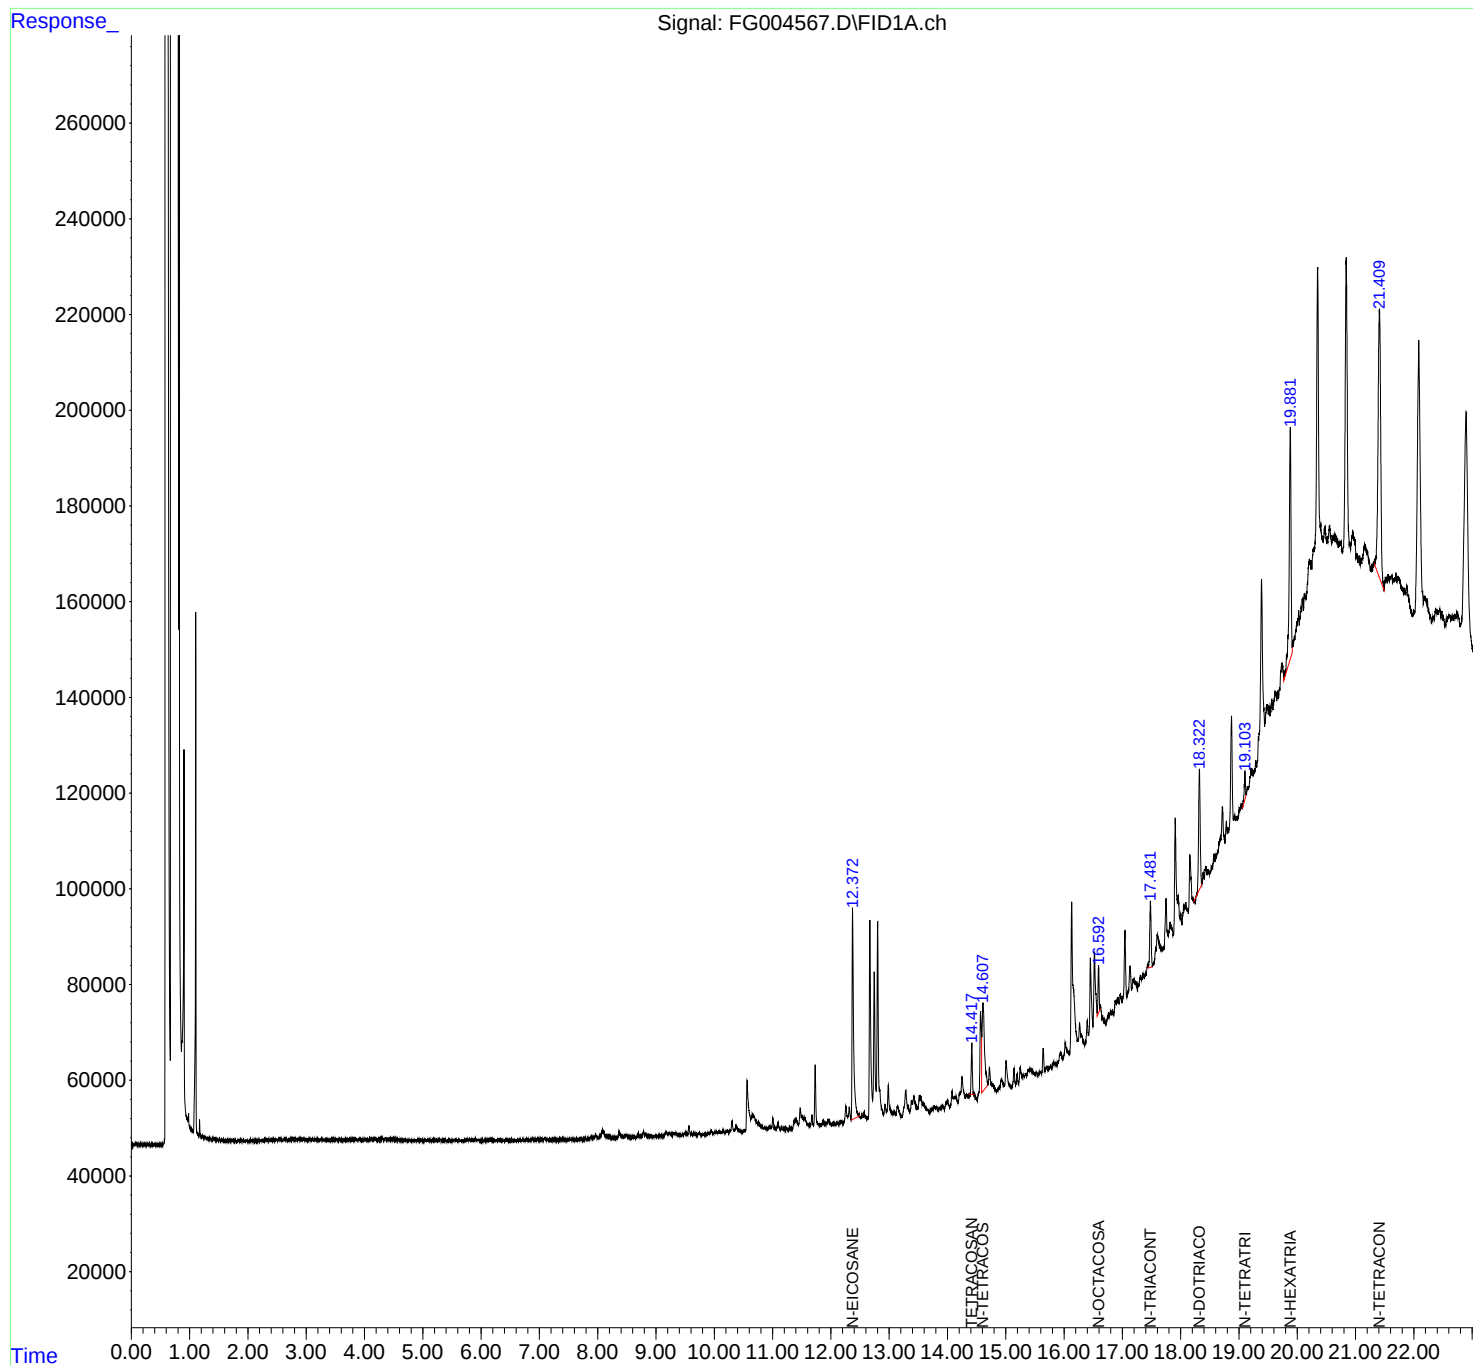


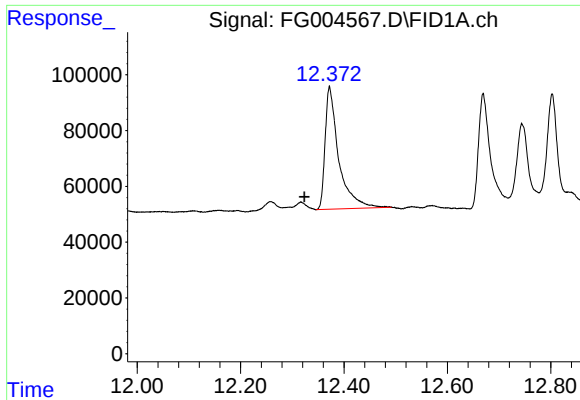

#7 N-EICOSANE


R.T.: 12.372 min
Delta R.T.: 0.049 min
Response: 800425
Conc: 7.00 ug/ml

Instrument :
FID_G
ClientSampleId :
SU-03-040219-B

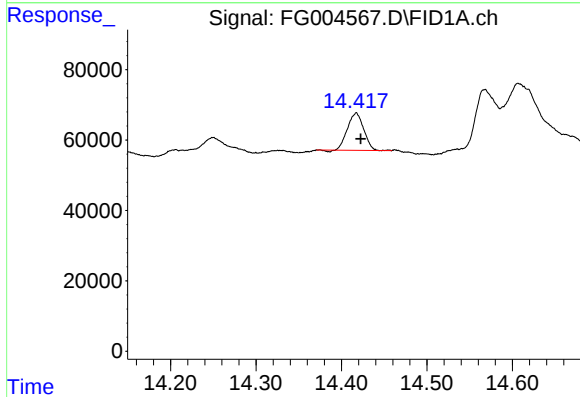


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.417 min
Delta R.T.: -0.005 min
Response: 140112
Conc: 1.36 ug/ml

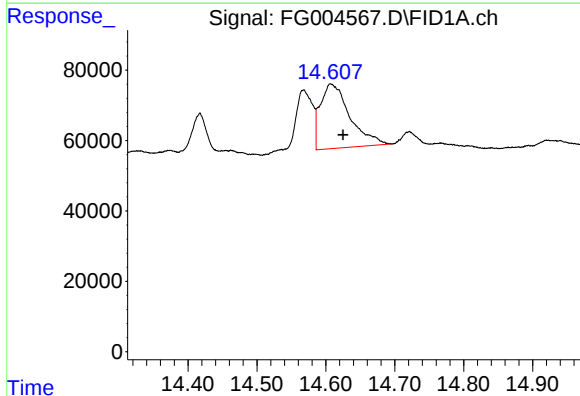


#10 N-TETRACOSANE

R.T.: 14.607 min
Delta R.T.: -0.018 min
Response: 544014
Conc: 4.71 ug/ml

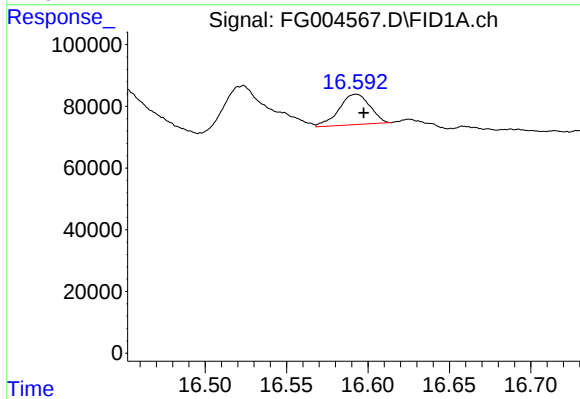

#12 N-OCTACOSANE


R.T.: 16.593 min
Delta R.T.: -0.005 min
Response: 130088
Conc: 1.12 ug/ml

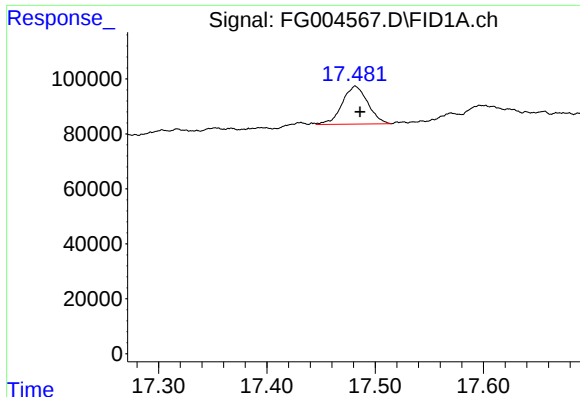

#13 N-TRIACONTANE


R.T.: 17.482 min
Delta R.T.: -0.004 min
Response: 225875
Conc: 1.90 ug/ml

Instrument :
FID_G
ClientSampleId :
SU-03-040219-B

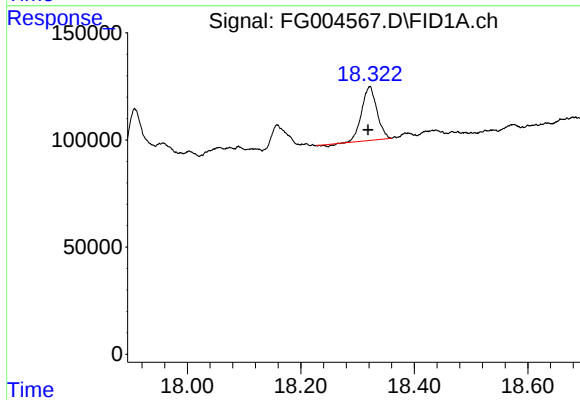


#14 N-DOTRIACONTANE

R.T.: 18.322 min
Delta R.T.: 0.003 min
Response: 462547
Conc: 3.94 ug/ml

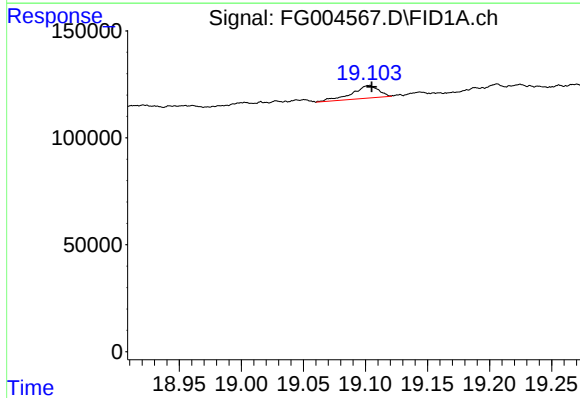


#15 N-TETRATRIACONTANE

R.T.: 19.103 min
Delta R.T.: -0.002 min
Response: 88148
Conc: 0.79 ug/ml

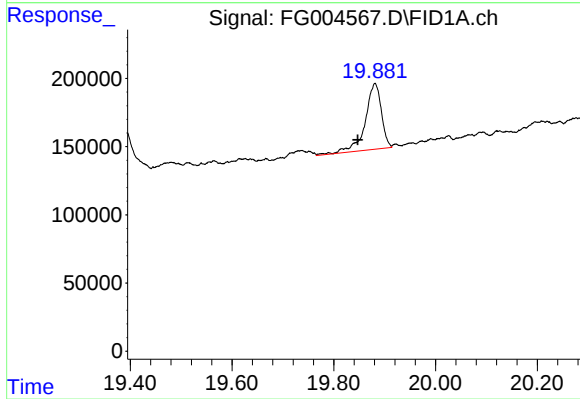

#16 N-HEXATRIACONTANE

R.T.: 19.881 min
Delta R.T.: 0.034 min
Response: 1066745
Conc: 9.57 ug/ml

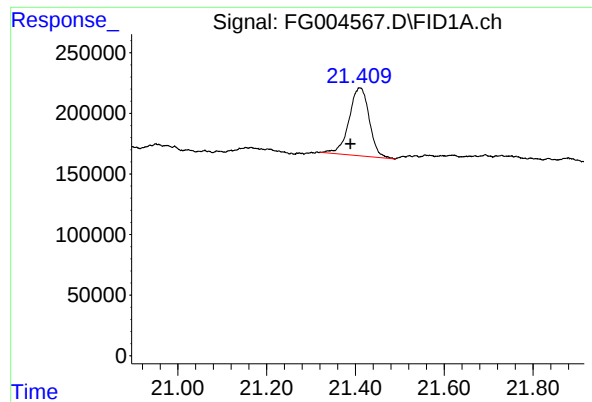

#18 N-TETRACONTANE

R.T.: 21.410 min
Delta R.T.: 0.021 min
Response: 1761800
Conc: 16.29 ug/ml

Instrument :
FID_G
ClientSampleId :
SU-03-040219-B