

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
 Data File : FG004582.D
 Signal(s) : FID1A.ch
 Acq On : 04 Apr 2019 10:20
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Apr 04 11:15:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.168	2900743	27.532 ug/ml
12) N-OCTACOSANE	16.590	3017042	26.079 ug/ml
13) N-TRIACONTANE	17.476	396625	3.343 ug/ml
14) N-DOTRIACONTANE	18.310	448172	3.822 ug/ml
15) N-TETRATRIACONTANE	19.094	325225	2.919 ug/ml
16) N-HEXATRIACONTANE	19.837	154513	1.386 ug/ml
17) N-OCTATRIACONTANE	20.548	127505	1.283 ug/ml
18) N-TETRACONTANE	21.392	162727	1.504 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004582.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 10:20
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 04 11:15:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

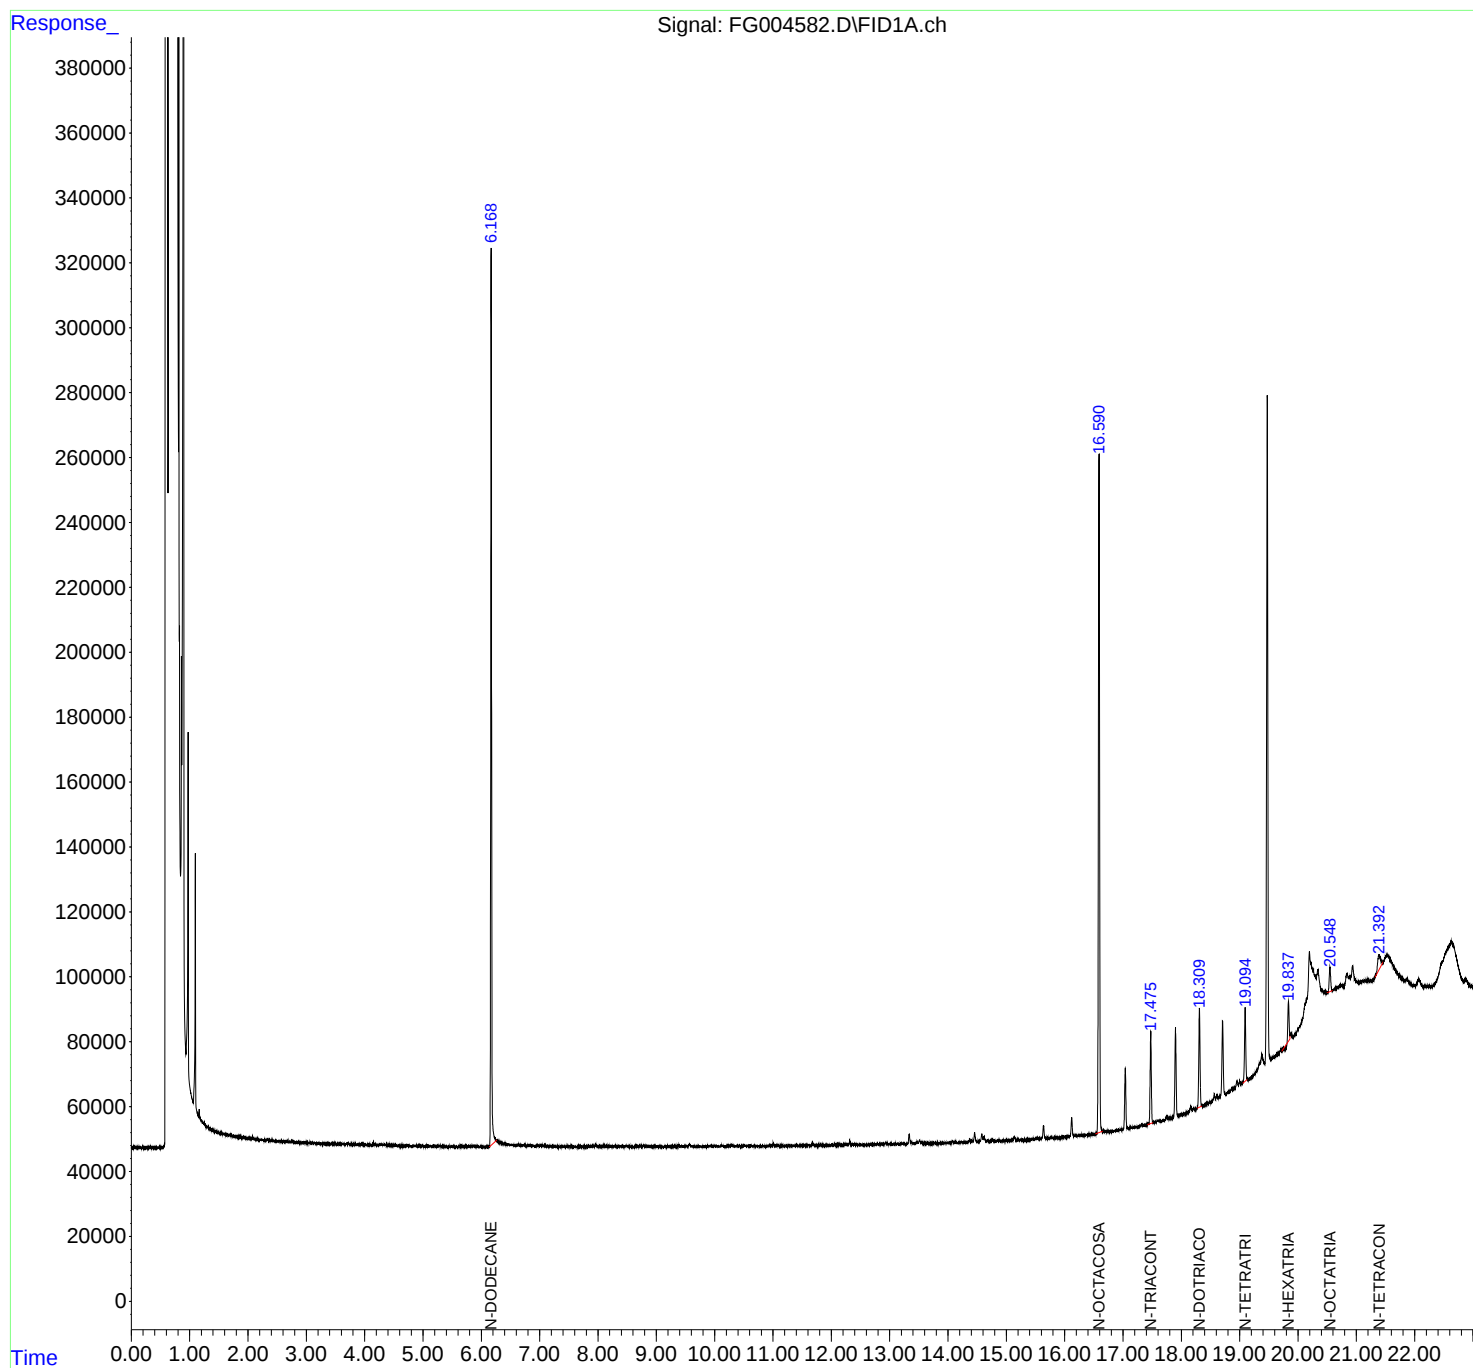


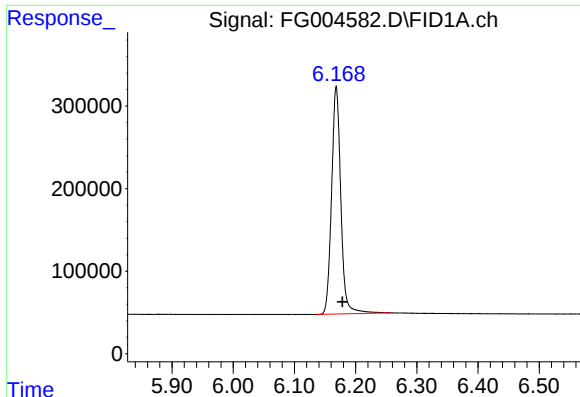

#3 N-DODECANE


R.T.: 6.168 min
Delta R.T.: -0.010 min
Response: 2900743
Conc: 27.53 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

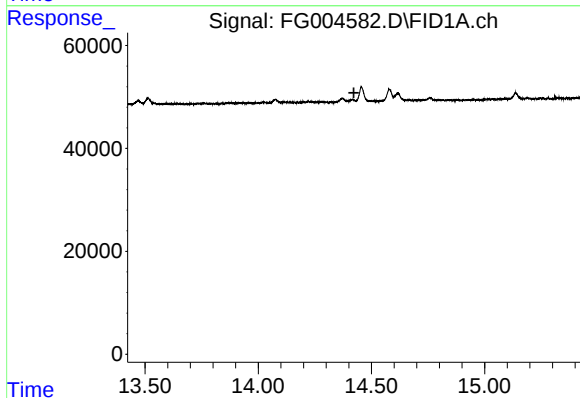


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

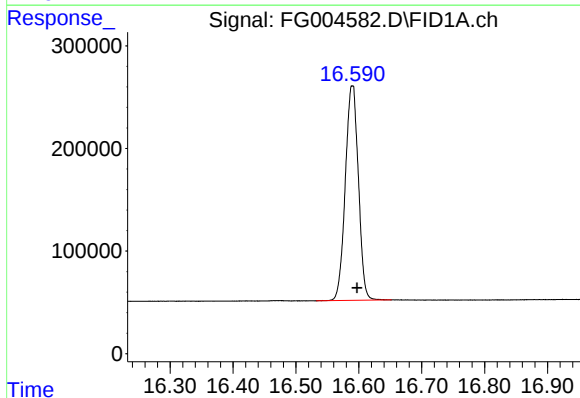


#12 N-OCTACOSANE

R.T.: 16.590 min
Delta R.T.: -0.008 min
Response: 3017042
Conc: 26.08 ug/ml

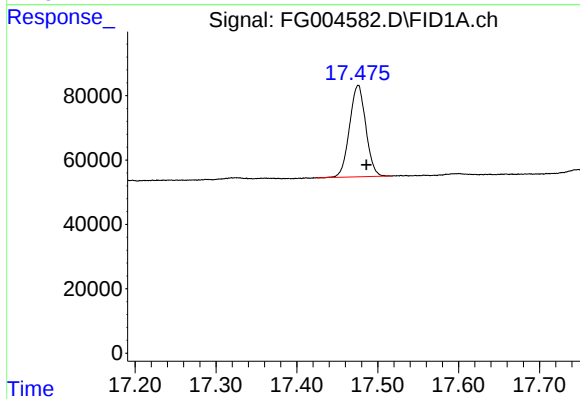

#13 N-TRIACONTANE


R.T.: 17.476 min
Delta R.T.: -0.010 min
Response: 396625
Conc: 3.34 ug/ml

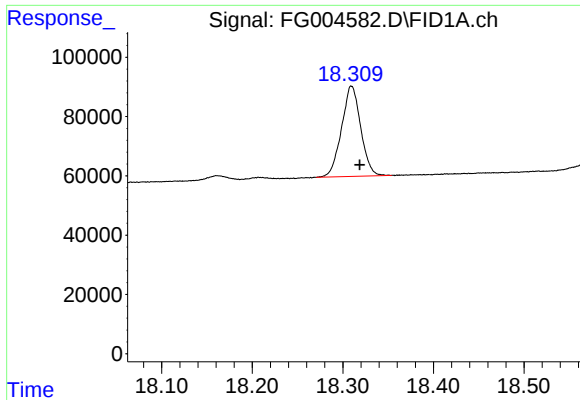

#14 N-DOTRIACONTANE


R.T.: 18.310 min
Delta R.T.: -0.009 min
Response: 448172
Conc: 3.82 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

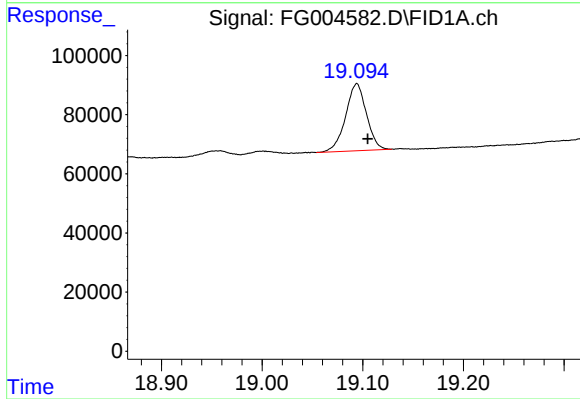


#15 N-TETRATRIACONTANE

R.T.: 19.094 min
Delta R.T.: -0.011 min
Response: 325225
Conc: 2.92 ug/ml

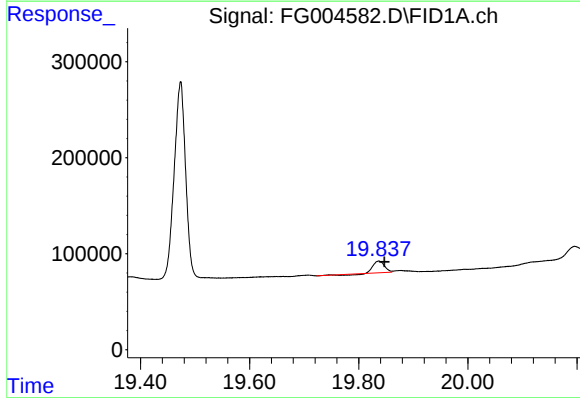


#16 N-HEXATRIACONTANE

R.T.: 19.837 min
Delta R.T.: -0.010 min
Response: 154513
Conc: 1.39 ug/ml

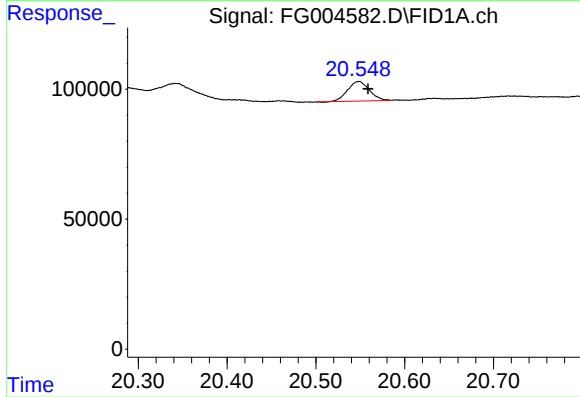

#17 N-OCTATRIACONTANE

R.T.: 20.548 min
Delta R.T.: -0.011 min
Response: 127505
Conc: 1.28 ug/ml

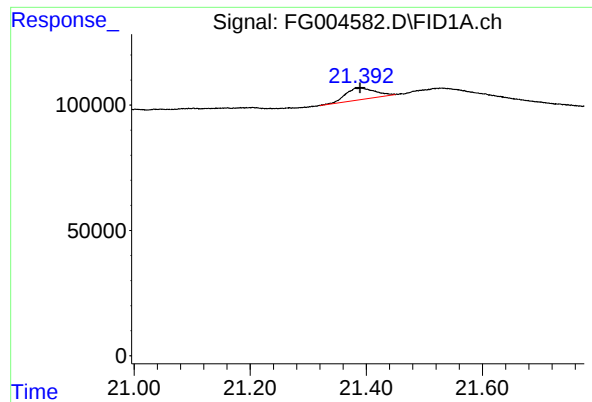

#18 N-TETRACONTANE

R.T.: 21.392 min
Delta R.T.: 0.003 min
Response: 162727
Conc: 1.50 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER