

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004584.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 11:21
Operator : AJ\SJ
Sample : K2197-03 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CL-02-040219-B

Integration File: autoint1.e
Quant Time: Apr 04 15:25:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.365	3821030	33.425 ug/ml
10)	N-TETRACOSANE	14.595	1751517	15.163 ug/ml
12)	N-OCTACOSANE	16.589	107070	0.926 ug/ml
13)	N-TRIACONTANE	17.475	115397	0.973 ug/ml
14)	N-DOTRIACONTANE	18.303	449571	3.834 ug/ml
15)	N-TETRATRIACONTANE	19.095	100717	0.904 ug/ml
16)	N-HEXATRIACONTANE	19.843	20909	0.188 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004584.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 11:21
Operator : AJ\SJ
Sample : K2197-03 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CL-02-040219-B

Integration File: autoint1.e
Quant Time: Apr 04 15:25:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

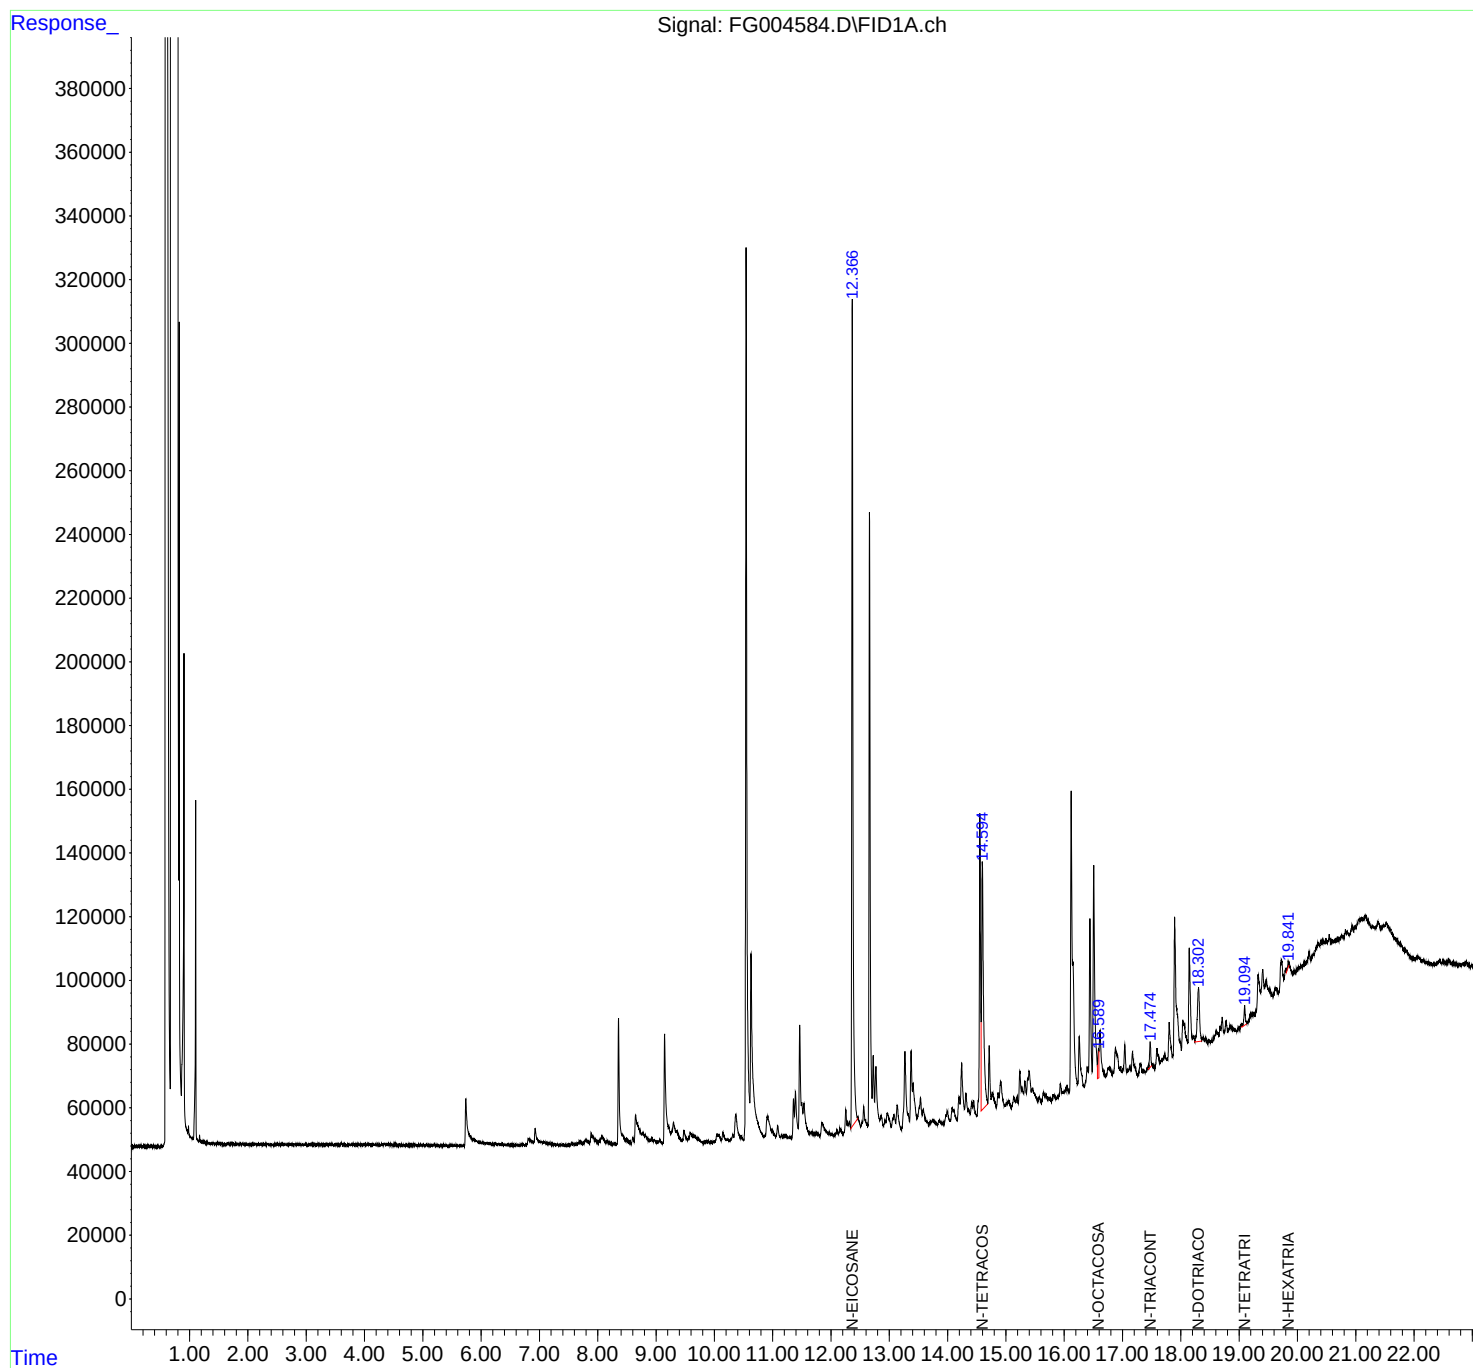


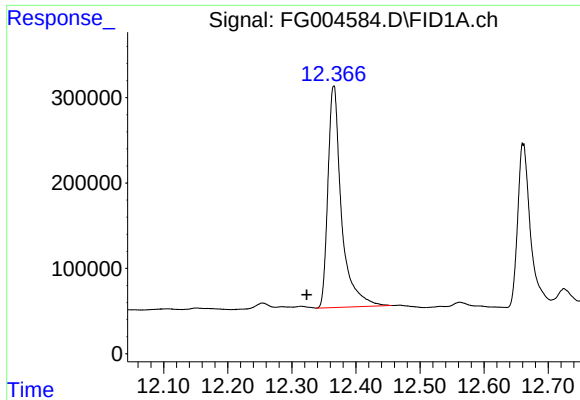

#7 N-EICOSANE


R.T.: 12.365 min
Delta R.T.: 0.042 min
Response: 3821030
Conc: 33.43 ug/ml

Instrument :
FID_G
ClientSampleId :
CL-02-040219-B

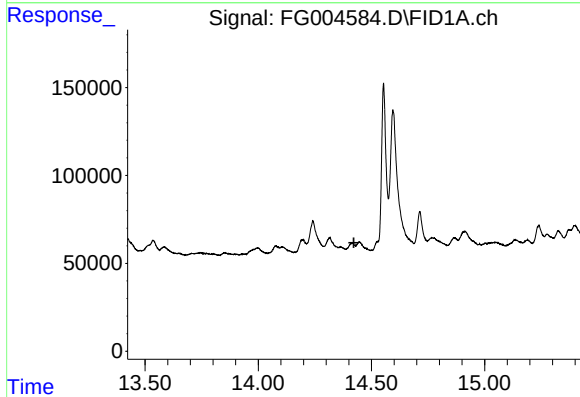


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.422 min
Response: 0
Conc: N.D.

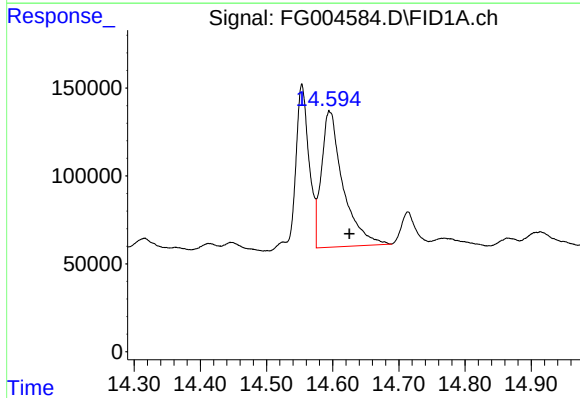


#10 N-TETRACOSANE

R.T.: 14.595 min
Delta R.T.: -0.030 min
Response: 1751517
Conc: 15.16 ug/ml

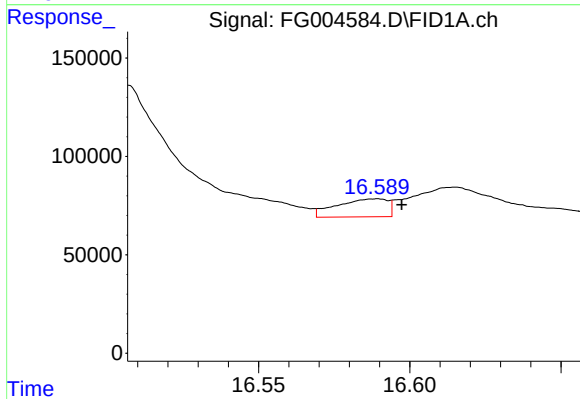

#12 N-OCTACOSANE


R.T.: 16.589 min
Delta R.T.: -0.008 min
Response: 107070
Conc: 0.93 ug/ml

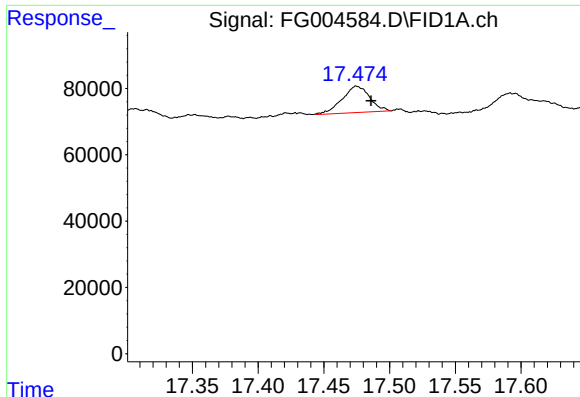

#13 N-TRIACONTANE


R.T.: 17.475 min
Delta R.T.: -0.011 min
Response: 115397
Conc: 0.97 ug/ml

Instrument :
FID_G
ClientSampleId :
CL-02-040219-B

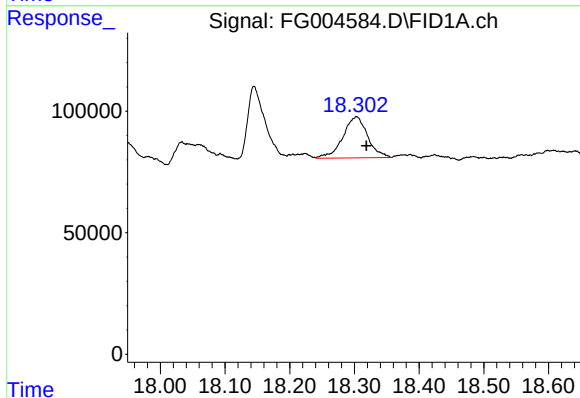


#14 N-DOTRIACONTANE

R.T.: 18.303 min
Delta R.T.: -0.015 min
Response: 449571
Conc: 3.83 ug/ml

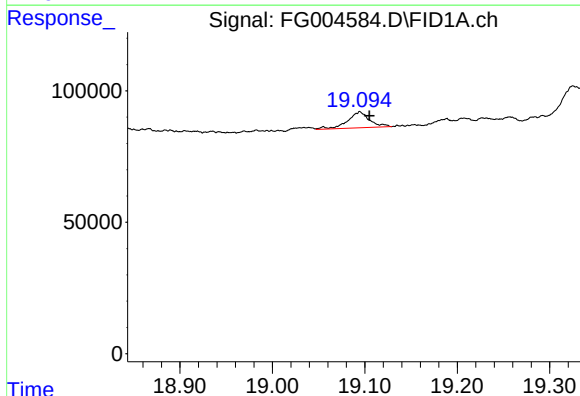

#15 N-TETRATRIACONTANE

R.T.: 19.095 min
Delta R.T.: -0.010 min
Response: 100717
Conc: 0.90 ug/ml

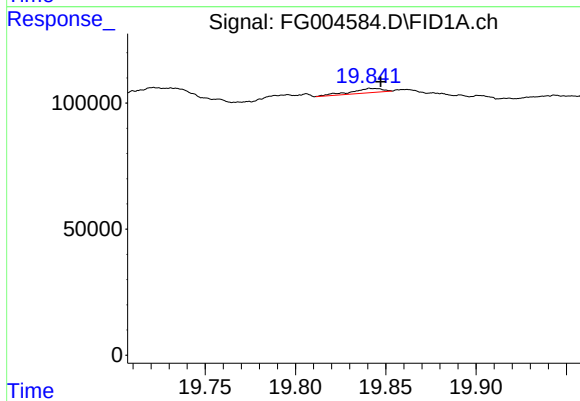

#16 N-HEXATRIACONTANE

R.T.: 19.843 min
Delta R.T.: -0.005 min
Response: 20909
Conc: 0.19 ug/ml