

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
 Data File : FG004585.D
 Signal(s) : FID1A.ch
 Acq On : 04 Apr 2019 11:52
 Operator : AJ\SJ
 Sample : K2199-01 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 OR-02-040219-A

Integration File: autoint1.e
 Quant Time: Apr 04 15:25:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.412	292381	2.835 ug/ml
Target Compounds			
6) N-OCTADECANE	11.003	82185	0.725 ug/ml
7) N-EICOSANE	12.369	718534	6.285 ug/ml
10) N-TETRACOSANE	14.608	558209	4.832 ug/ml
11) N-HEXACOSANE	15.638	126709	1.105 ug/ml
12) N-OCTACOSANE	16.589	161912	1.400 ug/ml
13) N-TRIACONTANE	17.476	419984	3.540 ug/ml
14) N-DOTRIACONTANE	18.311	267837	2.284 ug/ml
15) N-TETRATRIACONTANE	19.095	209469	1.880 ug/ml
16) N-HEXATRIACONTANE	19.839	172620	1.549 ug/ml
17) N-OCTATRIACONTANE	20.551	94980	0.956 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG040419\
Data File : FG004585.D
Signal(s) : FID1A.ch
Acq On : 04 Apr 2019 11:52
Operator : AJ\SJ
Sample : K2199-01 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OR-02-040219-A

Integration File: autoint1.e
Quant Time: Apr 04 15:25:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

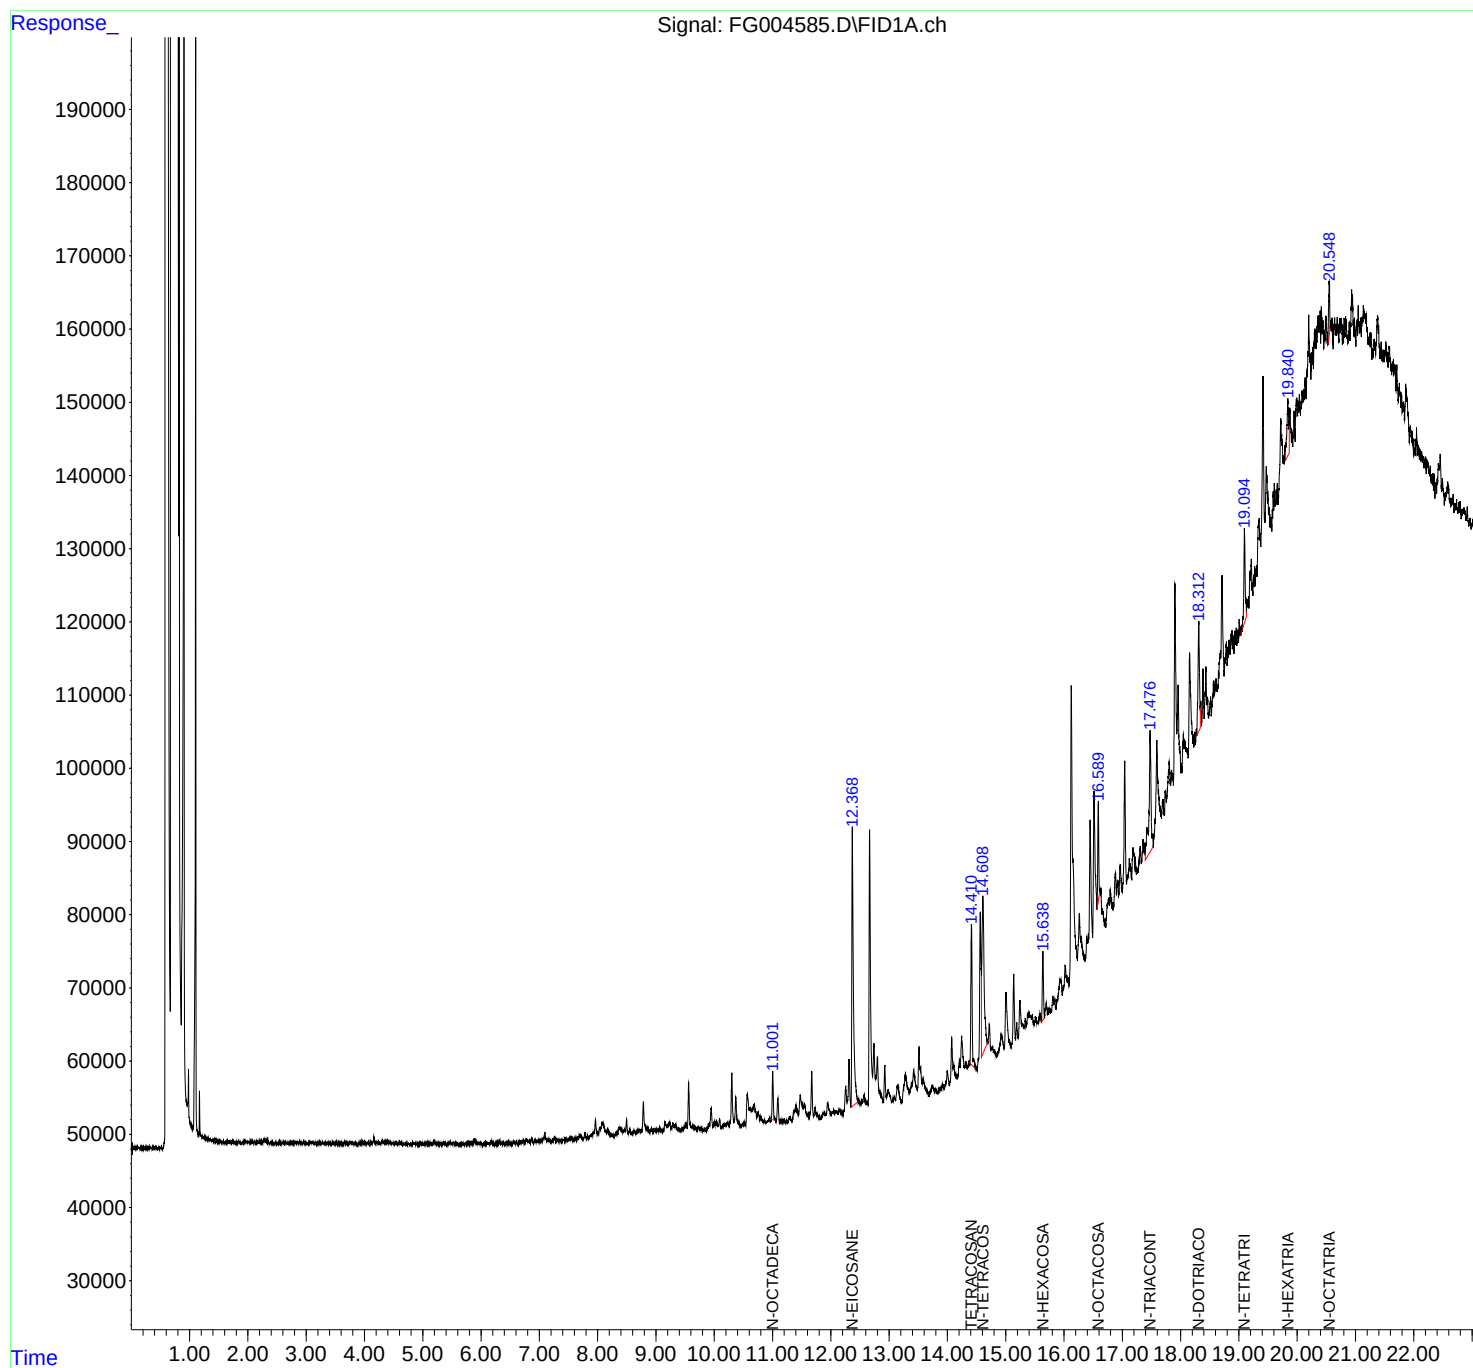


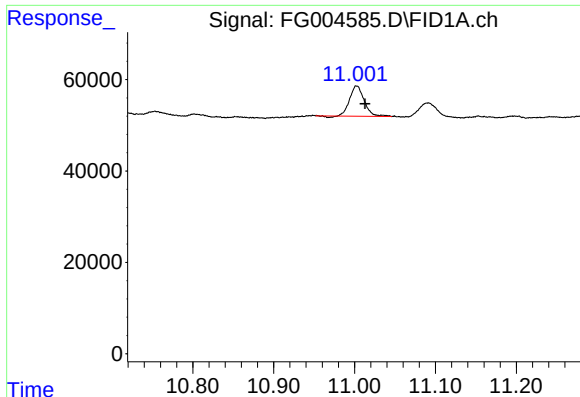

#6 N-OCTADECANE


R.T.: 11.003 min
Delta R.T.: -0.010 min
Response: 82185
Conc: 0.72 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-02-040219-A

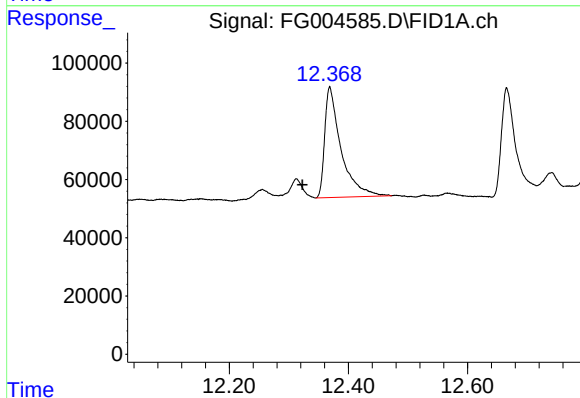


#7 N-EICOSANE

R.T.: 12.369 min
Delta R.T.: 0.046 min
Response: 718534
Conc: 6.29 ug/ml

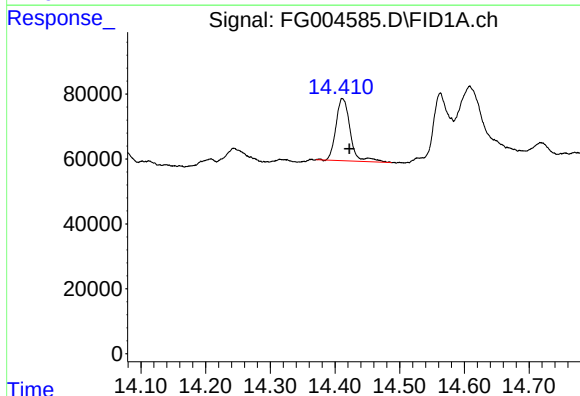


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.412 min
Delta R.T.: -0.011 min
Response: 292381
Conc: 2.83 ug/ml

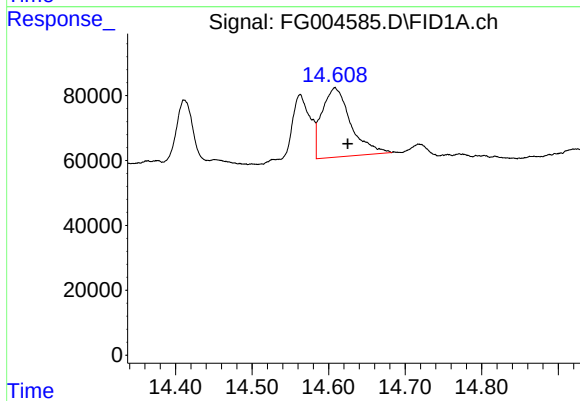

#10 N-TETRACOSANE


R.T.: 14.608 min
Delta R.T.: -0.017 min
Response: 558209
Conc: 4.83 ug/ml

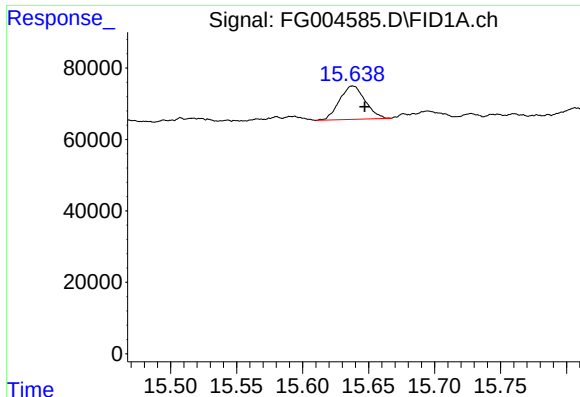

#11 N-HEXACOSANE


R.T.: 15.638 min
Delta R.T.: -0.009 min
Response: 126709
Conc: 1.11 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-02-040219-A

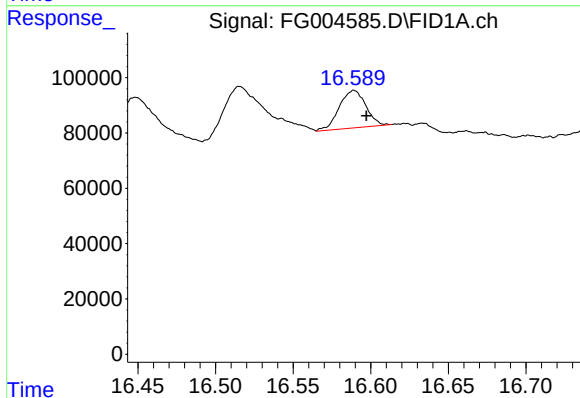


#12 N-OCTACOSANE

R.T.: 16.589 min
Delta R.T.: -0.008 min
Response: 161912
Conc: 1.40 ug/ml

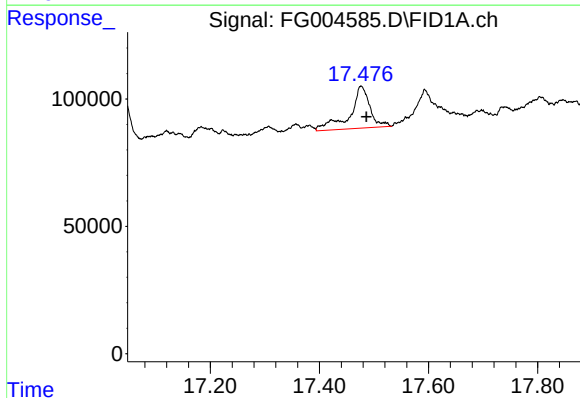


#13 N-TRIACONTANE

R.T.: 17.476 min
Delta R.T.: -0.010 min
Response: 419984
Conc: 3.54 ug/ml

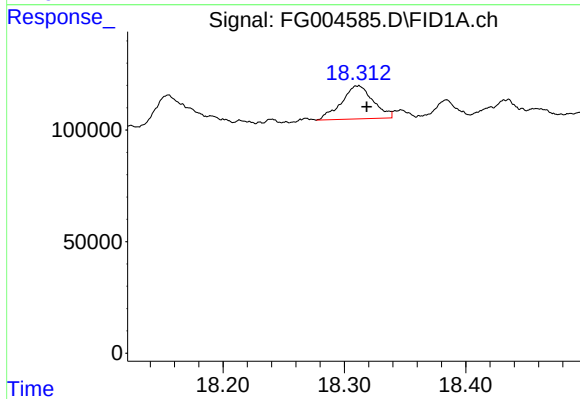

#14 N-DOTRIACONTANE


R.T.: 18.311 min
Delta R.T.: -0.007 min
Response: 267837
Conc: 2.28 ug/ml

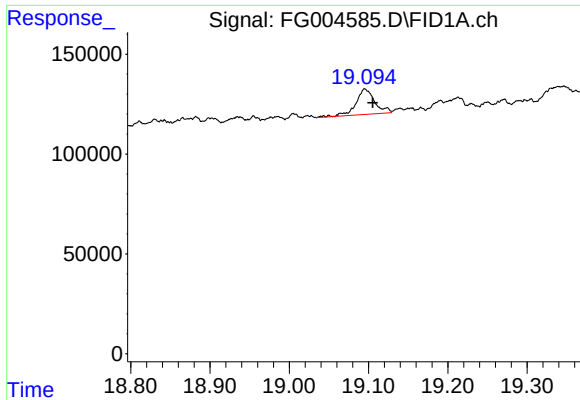

#15 N-TETRATRIACONTANE


R.T.: 19.095 min
Delta R.T.: -0.010 min
Response: 209469
Conc: 1.88 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-02-040219-A

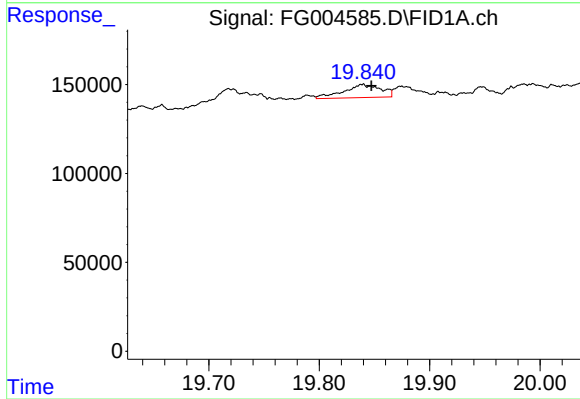

#16 N-HEXATRIACONTANE

R.T.: 19.839 min
Delta R.T.: -0.008 min
Response: 172620
Conc: 1.55 ug/ml

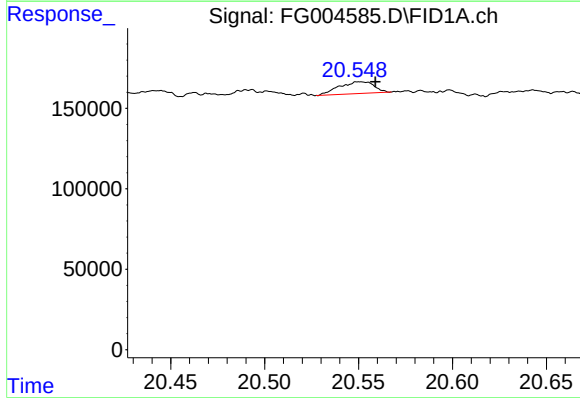

#17 N-OCTATRIACONTANE

R.T.: 20.551 min
Delta R.T.: -0.008 min
Response: 94980
Conc: 0.96 ug/ml